

- 30 Armentano RL, Santana DB, Cabrera Fischer EI, Graf S, Campos HP, German YZ, et al. An in vitro study of cryopreserved and fresh human arteries: a comparison with ePTFE prostheses and human arteries studied non-invasively in vivo. *Cryobiology* 2006;52:17–26.
- 31 Dorigo W, Pulli R, Castelli P, Dorrucchi V, Ferilli F, De Blasis G, et al. A multicenter comparison between autologous saphenous vein and heparin-bonded expanded polytetrafluoroethylene (ePTFE) graft in the treatment of critical limb ischemia in diabetics. *J Vasc Surg* 2011;54:1332–8.
- 32 Minga Lowampa E, Holemans C, Stiennon L, Van Damme H, Defraigne JO. Late fate of cryopreserved arterial allografts. *Eur J Vasc Endovasc Surg* 2016;52:696–702.
- 33 Kristensen SD, Knuuti J, Saraste A, Anker S, Botker HE, Hert SD, et al. 2014 ESC/ESA Guidelines on non-cardiac surgery: cardiovascular assessment and management: the Joint Task Force on non-cardiac surgery: cardiovascular assessment and management of the European Society of Cardiology (ESC) and the European Society of Anaesthesiology (ESA). *Eur Heart J* 2014;35:2383–431.
- 34 Liang NL, Baril DT, Avgerinos ED, Leers SA, Makaroun MS, Chaer RA. Comparative effectiveness of anticoagulation on midterm infrainguinal bypass graft patency. *J Vasc Surg* 2017;66:499–505.e2.

Eur J Vasc Endovasc Surg (2019) 57, 831


## COUP D’OEIL

### Type 1a Endoleak Secondary to Graft Migration

Yang Liu <sup>a,b</sup>, Yi Yang <sup>a,\*</sup>

<sup>a</sup>Department of Vascular Surgery, West China Hospital, Sichuan University, Chengdu, China

<sup>b</sup>West China School of Medicine, Sichuan University, Chengdu, China

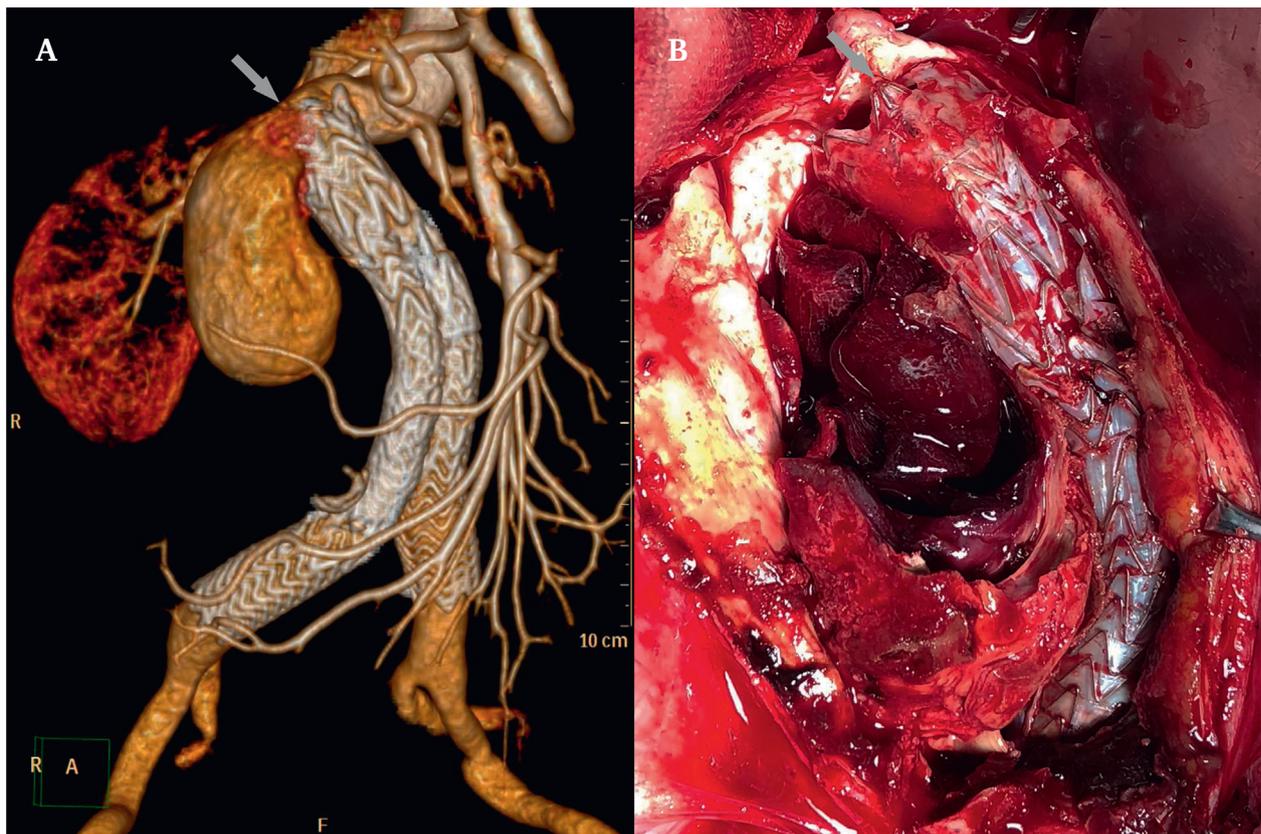

A 58 year old woman who underwent endovascular aneurysm repair one year previously for a 76 mm abdominal aortic aneurysm (AAA) with 70° neck angulation using locally made stent grafts (Percutek Therapeutics Co Ltd, Beijing, China), presented with severe acute abdominal pain. Computed tomographic angiography showed type 1a endoleak secondary to graft migration with AAA sac enlargement (panel A, grey arrow). The patient underwent emergency stent graft explantation (panel B) and aortic reconstruction with a 16 × 8 × 8 mm PTFE (polytetra-flour-ethylene) vascular prosthesis (GORE-TEX®, WL Gore & Associates, Flagstaff, USA). The patient made an excellent recovery with no complications at three-month follow-up.

\* Corresponding author. Department of Vascular Surgery, West China Hospital, Sichuan University, 37 Guo Xue Alley, Chengdu 610041, Sichuan Province, China.

E-mail address: [hallyangyi@126.com](mailto:hallyangyi@126.com) (Yi Yang).

1078-5884/© 2019 European Society for Vascular Surgery. Published by Elsevier B.V. All rights reserved.

<https://doi.org/10.1016/j.ejvs.2019.01.014>