

## Corrigendum

## Corrigendum to “3D printed bionic nanodevices” [Nano Today 11 (2016) 330–350]



Yong Lin Kong<sup>a,\*</sup>, Maneesh K. Gupta<sup>b</sup>, Blake N. Johnson<sup>c</sup>, Michael C. McAlpine<sup>d,\*</sup>


<sup>a</sup> Koch Institute for Integrative Cancer Research, Massachusetts Institute of Technology, Cambridge, MA 02139, USA

<sup>b</sup> Air Force Research Laboratories, Wright-Patterson Air Force Base, OH 45433, USA

<sup>c</sup> Department of Industrial and Systems Engineering, Virginia Tech, Blacksburg, VA 24061, USA

<sup>d</sup> Department of Mechanical Engineering, University of Minnesota, Minneapolis, MN 55455, USA

The authors regret there is a typo in Figure 3. The unit of the x-axis should be “ $\mu\text{m}$ ” rather than “mm”. This error occurred during editing, when the fonts were changed to “Arial” in Adobe Illustrator, in which the micron symbol ( $\mu$ ) is written with the “symbol” font of an “m” character. The corrected figure is included as followed:

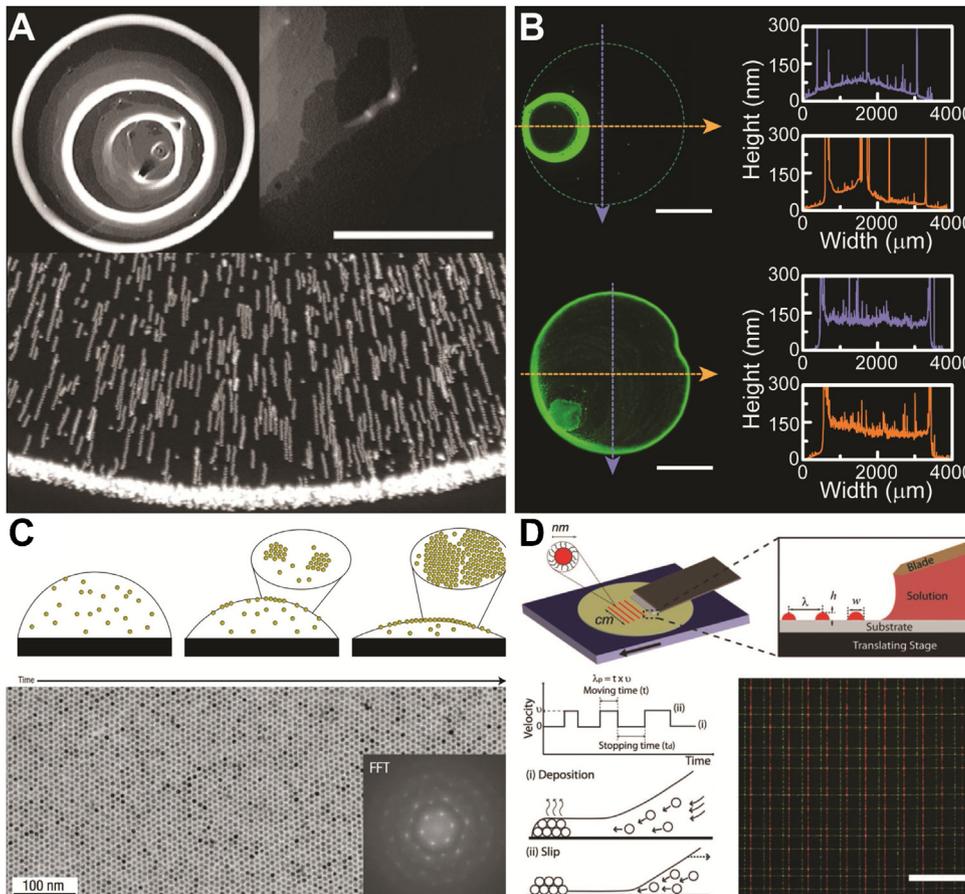

The authors would like to apologise for any inconvenience caused.

DOI of original article: <https://doi.org/10.1016/j.nantod.2016.04.007>.

\* Corresponding authors.

E-mail addresses: [yongkong@mit.edu](mailto:yongkong@mit.edu) (Y.L. Kong), [mcalpine@umn.edu](mailto:mcalpine@umn.edu) (M.C. McAlpine).

<https://doi.org/10.1016/j.nantod.2019.03.009>

1748-0132/© 2019 Elsevier Ltd. All rights reserved.