



Quantitative and rapid *Plasmodium falciparum* malaria diagnosis and artemisinin-resistance detection using a CMOS Lab-on-Chip platform



Kenny Malpartida-Cardenas^a, Nicholas Miscourides^a, Jesus Rodriguez-Manzano^{a,*},
Ling-Shan Yu^a, Nicolas Moser^a, Jake Baum^b, Pantelis Georgiou^a

^a Centre for Bio-Inspired Technology, Department of Electrical and Electronic Engineering, Imperial College London, UK

^b Department of Life Sciences, Imperial College London, UK

ARTICLE INFO

Keywords:

ISFET
CMOS
Lab-on-Chip
Point-of-Care
Malaria
P. falciparum
SNP
LAMP

ABSTRACT

Early and accurate diagnosis of malaria and drug-resistance is essential to effective disease management. Available rapid malaria diagnostic tests present limitations in analytical sensitivity, drug-resistance testing and/or quantification. Conversely, diagnostic methods based on nucleic acid amplification stepped forwards owing to their high sensitivity, specificity and robustness. Nevertheless, these methods commonly rely on optical measurements and complex instrumentation which limit their applicability in resource-poor, point-of-care settings. This paper reports the specific, quantitative and fully-electronic detection of *Plasmodium falciparum*, the predominant malaria-causing parasite worldwide, using a Lab-on-Chip platform developed in-house. Furthermore, we demonstrate on-chip detection of C580Y, the most prevalent single-nucleotide polymorphism associated to artemisinin-resistant malaria. Real-time non-optical DNA sensing is facilitated using Ion-Sensitive Field-Effect Transistors, fabricated in unmodified complementary metal-oxide-semiconductor (CMOS) technology, coupled with loop-mediated isothermal amplification. This work holds significant potential for the development of a fully portable and quantitative malaria diagnostic that can be used as a rapid point-of-care test.

1. Introduction

Rapid diagnosis of infectious diseases at the point-of-care (PoC) is essential to enable effective infection control, surveillance of cases and appropriate treatment administration (Vashist, 2017). Lab-on-chip (LoC) diagnostic platforms have experienced significant growth in recent years as the result of huge advances in several disciplines such as biosensing technologies, molecular biology and microfluidics. Their potential use in resource-limited settings while providing clinical sensitivity, specificity, high speed of detection and an easy-to-use interface are key factors for epidemiological reporting of antimicrobial-resistance, treatment and disease management (Kozel and Burnham-Marusich, 2017).

Various diagnostic techniques have been employed to identify the presence of pathogens in infected patients, targeting either the pathogen itself, biological products derived from the pathogen, or alterations in patients' biomolecules such as protein/nucleic acids. These techniques can be classified into three main categories: (i) cellular-based methods, (ii) protein-based methods and (iii) nucleic acid-based methods. Specifically, cellular-based methods such as microscopy, are

commonly used for pathogen identification, but require high expertise and expensive equipment thus limited to centralized facilities (Khan et al., 2016; Banoth et al., 2016; Hou et al., 2010; Lee et al., 2008; Wongsrichanalai et al., 2007). Conversely, most reported protein-based methods rely on antigen-antibody detection and are typically combined with paper-based diagnostics such as lateral flow assays (LFAs) (Moody, 2002; Hu et al., 2014; Krampa et al., 2017). Even though they report results within 5–15 min, they commonly suffer from low sensitivity or low specificity for clinical applications. In addition, they mainly rely on colorimetric or fluorescence measurements which are not usually capable of quantification unless expensive equipment such as optical cameras or lasers are involved (Obahiagbon et al., 2018). Instead, nucleic-acid amplification tests (NAATs) are characterized by high sensitivity and specificity, enabling quantification and detection of early stage infections. Among them, polymerase chain reaction (PCR) is the most widely used technique and is currently considered the gold standard in centralized laboratories. However, the requirements for thermal cycling and expensive equipment limit its application in PoC diagnostics. Instead, isothermal amplification methods have emerged as the next generation of NAATs due to their capability of running at constant

* Corresponding author.

E-mail address: j.rodriguez-manzano@imperial.ac.uk (J. Rodriguez-Manzano).

<https://doi.org/10.1016/j.bios.2019.111678>

Received 26 May 2019; Received in revised form 1 August 2019; Accepted 4 September 2019

Available online 07 September 2019

0956-5663/ © 2019 Elsevier B.V. All rights reserved.

temperature. In particular, loop-mediated isothermal amplification (LAMP) has received considerable attention due to its increased detection speed (less than 40 min) compared to PCR as well as higher specificity due to the use of 4–6 primers (as opposed to 2 in PCR) targeting 6–8 different genomic regions (Notomi et al., 2000). Nucleic acid amplification is facilitated by the strand displacement activity of the *Bst* DNA polymerase at 60°C–65°C. In this way, the need for thermal cycling to drive amplification is avoided and thus the instrumentation complexity and price are reduced. These features make LAMP an attractive NAAT method for the PoC diagnosis of infectious diseases (Rodriguez-Manzano et al., 2016; Wong et al., 2018; Yu et al., 2019).

One of the most threatening infectious diseases in resource-limited settings, malaria, with an estimated 219 million cases in 2017, has been highlighted by the World Health Organization (WHO) to be controlled or eliminated by 2030 (World Health Organization (WHO), 2019). Malaria is caused by the *Plasmodium* parasite, with five species identified to infect human population out of which *Plasmodium falciparum* is the most prevalent. In addition, the emergence of drug-resistant *P. falciparum* strains to medicines such as artemisinin, is compromising the effectiveness of current malaria treatments. Consequently, there is a significant need to specifically detect this pathogen with high sensitivity and rapid detection for adequate therapy prescription and epidemiological surveillance. Most rapid diagnostic tests developed for this purpose are no longer reliable due to the loss of expression of targeted proteins, such as HRP-II (leading to high occurrence of false negatives) (Beshir et al., 2017; Cheng et al., 2014). As a result, subsequent efforts have focused their attention on NAATs, primarily targeting the gene *18S rRNA*. Nevertheless, significant challenges towards PoC diagnosis still exist with (i) gold standards being PCR-based which rely on thermal cycling and reported time-to-results longer than 1 h, (ii) most of the reported LAMP primer sets (Mohon et al., 2014; Lau et al., 2016; Han et al., 2007) did not consider the zoonotic *Plasmodium* species which have recently jumped to infect human hosts (Moon et al., 2013; Bronner et al., 2009), (iii) most of the reported NAATs are lab-based and non applicable in the field and (iv) if targeting PoC applications, they commonly rely on optical measurements which typically only provide qualitative results. A summary of the most relevant NAATs for *P. falciparum* identification is provided in Table 1.

As opposed to optical-based detection, electrochemical detection is more promising due to innate capabilities such as high sensitivity, large scale integration, detection on miniaturized hardware, fast response and quantifiable measurements (Kurbanoglu et al., 2016; Labuda et al.,

2010). Field-effect transistors and more specifically ion-sensitive field-effect transistors (ISFETs) are emerging potentiometric sensors for NAAT applications. Owing to their compatibility with CMOS (complementary metal-oxide-semiconductor) technology, fully-electronic chemical detection is possible while ensuring sensor miniaturisation, mass manufacturing and low cost. CMOS-based ISFET sensing has been previously demonstrated for the detection of DNA amplification by employing an adapted version of LAMP, called pH-LAMP, that allows changes in pH to occur during nucleic acid amplification such that they can be detected by the ISFET sensors (Toumazou et al., 2013; Moser et al., 2018; Miscourides et al., 2018; Cacho-Soblechero et al., 2019). Furthermore, this technology is a suitable candidate for point-of-care implementations through transferring the amplification chemistries on a Lab-on-Chip platform with integrated sensing.

In this paper, we report the rapid and specific detection of *P. falciparum* malaria using a novel molecular assay targeting the gene *kelch 13*. Detection takes place in less than 20 min in isothermal conditions using LAMP. Furthermore, we show pH-LAMP based detection of malaria on a Lab-on-Chip platform which uses ISFETs to facilitate direct chemical-to-electronic sensing. The LoC platform demonstrates for the first time DNA quantification on-chip, using DNA samples derived from clinical isolates of *P. falciparum*. In addition, we further demonstrate on the LoC platform detection of the *C580Y* single-nucleotide polymorphism (SNP) associated with artemisinin-resistant malaria. Overall, the proposed molecular methods in combination with ISFET-based sensing are capable of label-free amplification and quantification of nucleic acids and thus lend themselves to PoC implementations of any desired target (including both DNA and RNA) with high sensitivity, specificity and speed of detection.

2. Materials and methods

2.1. Molecular methods

2.1.1. LAMP primer design specific to *P. falciparum*

A LAMP primer set for the detection of the gene *Kelch 13* of *P. falciparum*, named LAMP-PfK13, was designed based on the alignment of consensus reference genomic sequences. These included all human-infective *Plasmodium* species and some zoonotic *Plasmodium* species, such as *P. knowlesi* and *P. cynomolgi* which have recently jumped to infect human hosts (Bronner et al., 2009; Law, 2018). Sequences were retrieved from *Plasmodium* Genomic Resource (PlasmoDB) (Aurrecochea

Table 1
Nucleic-acid amplification tests for the specific detection of *P. falciparum*.

Assay	Target (gene)	Limit of Detection	Time to Positive	Species considered	Ref.
Nested PCR	18S rRNA	6 p/μL ^a	> 60 min	Pv, Po, Pm*	Singh et al., 1999
Nested PCR	K13	NA ^b	> 60 min	Pv, Po, Pm, Pk	Talundzic et al., 2015
PCR	18S rRNA	1 c/r	> 60 min	Pv, Po, Pm	Mangold et al., 2005
LAMP	18S rRNA	100 c/r ^c	32 min	Pv, Po, Pm	Han et al., 2007
LAMP	18S rRNA	5 p/μL	35 min	Pv, Pm*	Mohon et al., 2014
LAMP	18S rRNA	100 p/μL	> 60 min	Pv, Po, Pm*	Poon et al., 2006
LAMP	18S rRNA	1 c/r	35 min	Pv, Po, Pm, Pk*	Lau et al., 2016
LAMP	mitochondrial ^d	5 p/μL	30–40 min	Pv, Po, Pm, Pk	Polley et al., 2010
LAMP ^e	ND ^f	1 p/μL	45 min	ND ^f	Worldwide, 2019
LAMP ^g	K13	1 c/r	< 20 min	Pv, Po, Pm, Pk	This work
pH-LAMP ^g	K13	10 c/r	< 25 min	Pv, Po, Pm, Pk	This work

* *Plasmodium* species mentioned in the corresponding manuscript, with no cross-reactivity results among species shown.

^a Parasites per μL of blood (p/μL).

^b Not Available.

^c Copies per reaction (c/r).

^d DNA.

^e Qualitative.

^f Non Disclosed.

^g Quantitative. This table displays information as stated in company websites, product specification sheet, or references and does not intend to cover all nucleic-acid diagnostic tests for *P. falciparum* detection.

et al., 2009) and aligned using the MUSCLE algorithm (Edgar, 2004) in Geneious 10.0.5 software (Kearse et al., 2012). Gene IDs of the sequences used for the alignment can be found in Fig. S1. The LAMP primer set LAMP-PfK13 was designed using Primer Explorer V5¹ and optimised manually to ensure specificity. The LAMP-PfK13 primer set spans an amplicon size of 219 bp and consists of 6 primers targeting 8 different regions: two outer primers F3 and B3, two loop primers LF and LB and two inner primers FIP and BIP. Sequences of the primers can be found in Table S1.

2.1.2. Reaction conditions

Each LAMP reaction contained the following: 1.5 μL of $10 \times$ isothermal buffer (New England Biolabs),² 0.9 μL of MgSO_4 (100 mM stock), 2.1 μL of dNTPs (10 mM stock), 0.375 μL of BSA (20 mg/mL stock), 2.4 μL of Betaine (5M stock), 0.375 μL of SYTO 9 Green (20 μM stock), 0.6 μL of Bst 2.0 DNA polymerase (8000 U/mL stock), 3 μL of different concentrations of synthetic DNA or gDNA, 1.5 μL of $10 \times$ LAMP primer mixture (20 μM of BIP/FIP, 10 μM of LF/LB, and 2.5 μM B3/F3) and enough nuclease-free water (ThermoFisher Scientific) to bring the volume to 15 μL . Reactions were performed at 63°C for 35 min. One melting cycle was performed at 0.1 °C/s from 65°C up to 97°C for validation of the specificity of the products. Experiments were carried out in triplicates (5 μL each reaction) loading the reactions into LightCycler Multiwell Plates 96 (Roche Diagnostics) utilising a LightCycler 96 Real-Time PCR System (Roche Diagnostics). All primers used in this study were purchased from Integrated DNA Technologies.

In order to transfer amplification chemistries on a Lab-on-Chip platform, they need to be compatible with the sensing capabilities of ISFET sensors. Since ISFETs are intrinsically pH sensors (mechanism for pH sensitivity elaborated in Section 2.2), the reaction mix of standard LAMP was modified to pH-LAMP. In this case, the buffering conditions were adjusted such that pH changes could be measured. Each reaction contained the following: 3.0 μL of $10 \times$ isothermal customized buffer (pH 8.5–9), 1.8 μL of MgSO_4 (100 mM stock), 4.2 μL of dNTPs (10 mM stock), 1.8 μL of BSA (20 mg/mL stock), 4.8 μL of Betaine (5M stock), 1.88 μL of Bst 2.0 DNA polymerase (8000 μM /mL stock), 3 μL of different concentrations of synthetic DNA or gDNA, 0.75 μL of NaOH (0.2 M stock), 3 μL of $10 \times$ LAMP primer mixture, 0.75 μL of SYTO 9 Green (20 μM stock) only for qPCR experiments, and enough nuclease-free water (ThermoFisher Scientific) to bring the volume to 30 μL . Experiments were conducted in triplicates (10 μL each).

2.1.3. Samples and DNA extraction methods

A gBlock Gene fragment (synthetic DNA) containing the *kelch 13* region of interest was purchased from Integrated DNA Technologies and re-suspended in TE buffer to 5 ng/ μL stock solution, stored at -20°C until further use. *Plasmodium* extracted genomic DNA (gDNA) of all *Plasmodium* species known to infect humans (*P. falciparum*, *P. ovale curtisi*, *P. ovale wallikeri*, *P. vivax*, *P. malariae* and *P. knowlesi*) were included in the sample set.³ *P. falciparum* extracted genomic gDNA samples containing the Y493H mutation (ANL8G), and the C580Y mutation (ANL5G) in the gene *kelch 13* were isolated from Cambodian isolates using the PureLink Genomic DNA Mini Kit (ThermoFisher Scientific).

2.1.4. Analytical sensitivity

The sensitivity of the LAMP-PfK13 primer set was evaluated using ten-fold serial dilutions of synthetic DNA ranging from 1×10^7 to 1×10^0 copies per reaction with LAMP and pH-LAMP. For each method, a standard curve was obtained by plotting the time to positive

(TTP) against copies per reaction accompanied by the standard deviations.

2.1.5. Cross-reactivity and detection of clinical isolates

Ten DNA samples derived from clinical isolates were tested with the LAMP-PfK13 primer set to prove the absence of cross-reactivity with any other human-infective *Plasmodium* species. Samples (gDNA) included: *P. ovale curtisi*, *P. ovale wallikeri*, *P. vivax*, *P. malariae*, two *P. knowlesi* samples and four *P. falciparum* samples with one harbouring the mutant allele 580Y, one harbouring the mutant allele 493H, and two wild type samples.

2.1.6. SNP discrimination on-chip

In the case of specific SNP detection, mutant (MT) and wild-type (WT) reactions were performed as described in Malpartida-Cardenas et al. (2018). Sequences of primers can be found in Table S6. These reactions consisted of SNP-based LAMP (sbLAMP) primers targeting the specific allele for amplification (i.e MT allele), and unmodified self-stabilising (USS) competitive primers targeting the other allele (i.e WT allele) to robustly delay or prevent unspecific amplification. Each USS-sbLAMP reaction followed the usual LAMP reaction protocol with the inclusion of $10 \times$ sbLAMP primer mixture (20 μM of sbBIP/sbFIP, 10 μM of LF/LB, 2.5 μM B3/F3 and 30 or 40 μM of FB/BB). USS primers were re-suspended in TE buffer to 400 μM . Reactions were carried-out at 63°C for 35 min. This method was modified to be pH-sensitive such that it could be utilised in combination with the LoC platform as described in Section 2.1.2.

2.1.7. Gel electrophoresis

Agarose gels were prepared at 1.5% w/v with TBE $1 \times$ buffer and SYBR Safe DNA Gel Stain 1000 \times . LAMP products were mixed with loading dye (#B7024S, New England BioLabs) at $6 \times$ concentration prior to loading into pre-cast wells in the gel. As reference, 100 bp DNA ladder (#10488058, Invitrogen) was loaded. Power supply was set at 140 V to run the gel for 1 h. Stained DNA was visualized under UV light with UV BioSpectrum Imaging System instrument (Ultra-Violet Products Ltd.).

2.1.8. Statistical analysis

Time-to-positive data is presented as mean TTP \pm standard deviation; p-values were calculated by Student's heteroscedastic t-test with a two-sided distribution. Statistically significant difference was considered as: *p-value < 0.05, **p-value < 0.01, ***p-value < 0.001 and ****p-value < 0.0001. Correlation coefficients were calculated using Eq. (1) in Table S2.

2.2. CMOS-based chemical sensing

2.2.1. ISFET-based sensing

Detecting pH changes in an electrochemical manner is facilitated using ISFETs fabricated in unmodified CMOS technology (Georgiou and Toumazou, 2009). ISFETs are designed the same way as MOSFETs (metal-oxide-semiconductor field-effect transistors) with the gate extended to the top metal layer using a floating metal stack. With this method, the gate is biased using a reference electrode (typically Ag/AgCl) immersed in a solution. Sensing takes place through the passivation layer or the deposition of a suitably selective membrane which exhibits site binding and develops a double layer capacitance when exposed to an aqueous solution. The accumulation of protons due to the combined effect of the electrode biasing and the hydrogen ion concentration in the solution is capacitively coupled to the floating gate and modulates the gate potential of the underlying device. When biased with a stable reference electrode voltage, variations at the floating gate potential can be attributed to changes in ion concentration in the solution therefore a pH dependence is observed.

The equivalent circuit macromodel of an ISFET in unmodified

¹ Eiken Chemical Co. Ltd., Tokyo, Japan, <http://primerexplorer.jp/lampv5e/index.html>.

² Catalogue number B0537S.

³ These samples were kindly provided by Prof. Colin Sutherland from The London School of Hygiene and Tropical Medicine.

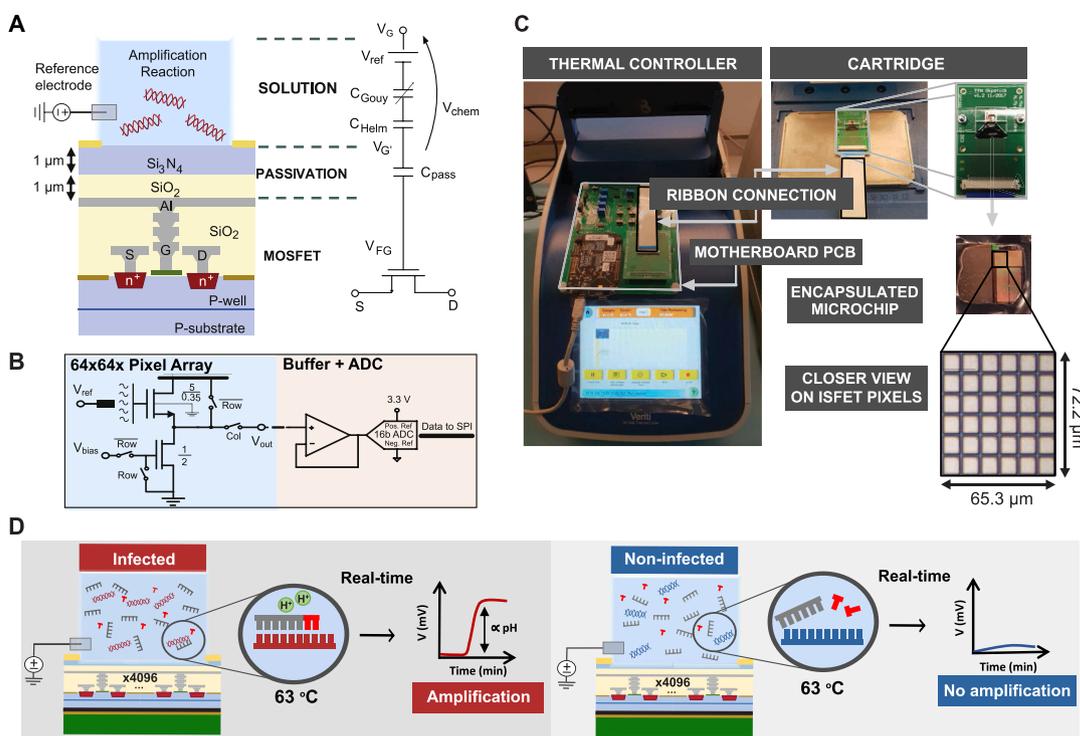


Fig. 1. Experimental configuration using the Lab-on-Chip platform. (A) Cross-section of an ISFET fabricated in unmodified CMOS technology and equivalent circuit macromodel. (B) Schematic of the pixel circuit implemented as a source follower configuration where changes in V_{out} reflect changes in pH (Miscourides and Georgiou, 2019). (C) Setup showing the Lab-on-Chip (LoC) platform including a motherboard PCB that facilitates data readout, a cartridge PCB hosting the microchip and microfluidic chamber, the microchip including an array of 4096 ISFET sensors and an external thermal controller. Furthermore, a microphotograph showing a 6×6 subset of the ISFET array. (D) Cross-section illustration of the LoC platform showing the reaction interface. Amplification at 63°C only occurs if the specific target is present in the loaded sample. Results are displayed in real-time.

CMOS technology is shown in Fig. 1A with the chemical dependence described by a term called V_{chem} (Georgiou and Toumazou, 2009) given by:

$$V_{chem} = \gamma + 2.3\alpha U_T \text{pH} \quad (1)$$

where γ describes all the constant terms not related to pH, α is a dimensionless sensitivity parameter and U_T is the thermal voltage.

Owing to their compatibility with modern electronic processes and the economies of scale of silicon, ISFET-based sensing has the potential for miniaturized, mass-fabricated and low-cost solutions. As a result, microchips with integrated ISFET sensing provide an attractive silicon substrate for LoC applications. However, sensor non-idealities exist which impose additional challenges on chemical sensing in unmodified CMOS (Liu et al., 2011). Firstly, trapped charge is typically left during fabrication at the floating gate and manifests as a random offset across sensors. This can be compensated by introducing sensor redundancy to reduce the susceptibility to high offsets and ensuring a large dynamic range in which sensors operate linearly irrespective of offsets. Secondly, the sensing membrane undergoes hydration after being exposed to an aqueous solution which manifests as a slow change on the output signal, typically referred to as drift. Drift is typically slower than pH changes due to DNA reaction dynamics and generic compensation methods have typically revolved around derivative-based methods (Jamasb, 2004). In this case, a compensation method was developed and is described in Section 2.4 to decouple the local changes in pH from the background drift.

2.2.2. ISFET sensing array

An array of 64×64 ISFET pixels of identical geometry has been fabricated in a commercial (AMS $0.35 \mu\text{m}$) CMOS process using silicon nitride (Si_3N_4) as the passivation (sensing) layer. Each pixel includes an ISFET configured in a source follower topology as shown in Fig. 1B with

the pixel's output buffered and sampled using an external 16-b ADC. This way changes in pH are linearly converted into changes in V_{out} for active pixels in the linear input range i.e. excluding extreme cases of trapped charge. Each pixel spans approximately $96 \mu\text{m}^2$ of silicon area with the total array of 4096 sensors spanning 0.56mm^2 . The intrinsic pH sensitivity of the Si_3N_4 layer has been measured to be 18mV/pH with the final sensitivity of V_{out} to pH after capacitive attenuation measured to be $S_{pH} = \frac{dV_{out}}{dpH} = -9.23 \text{mV/pH}$. A detailed description of the circuit design, instrumentation pipeline and method to derive the pH sensitivity is provided in (Miscourides and Georgiou, 2019).

2.2.3. Experimental setup for Lab-on-Chip reactions

To facilitate data readout and communication to a PC, a printed-circuit-board (PCB) was designed to host a microcontroller serving as an intermediary node between the microchip and a PC as shown in Fig. 1C. Furthermore, a separate cartridge PCB was designed to host the microchip which is connected with a ribbon cable to the main PCB and communication takes place via the serial peripheral interface. A Matlab-based graphical user interface is used to control all operations and provide real-time data recording and visualisation at 0.3 fps.

Moving towards a LoC platform to carry out on-chip DNA amplification detection, a microfluidic reaction chamber was laser cut from a 3 mm acrylic sheet and assembled on top of the CMOS microchip. In addition, an Ag/AgCl reference electrode was inserted in the chamber for sensor biasing, which was obtained by chlorination of a 0.03 mm diameter Ag wire in 1M KCl. To carry-out DNA amplification reactions, the microfluidic chamber was filled with $13 \mu\text{L}$ of pH-LAMP or pH-USS-sbLAMP reagents and sealed with PCR tape to avoid evaporation and contamination of the amplified products. Subsequently, the cartridge PCB was placed on top of a thermal cycler (Veriti Thermal Cycler, Applied Biosystems) used as a temperature controller to keep the solution at 63°C for isothermal amplification. After 35 min, the solution

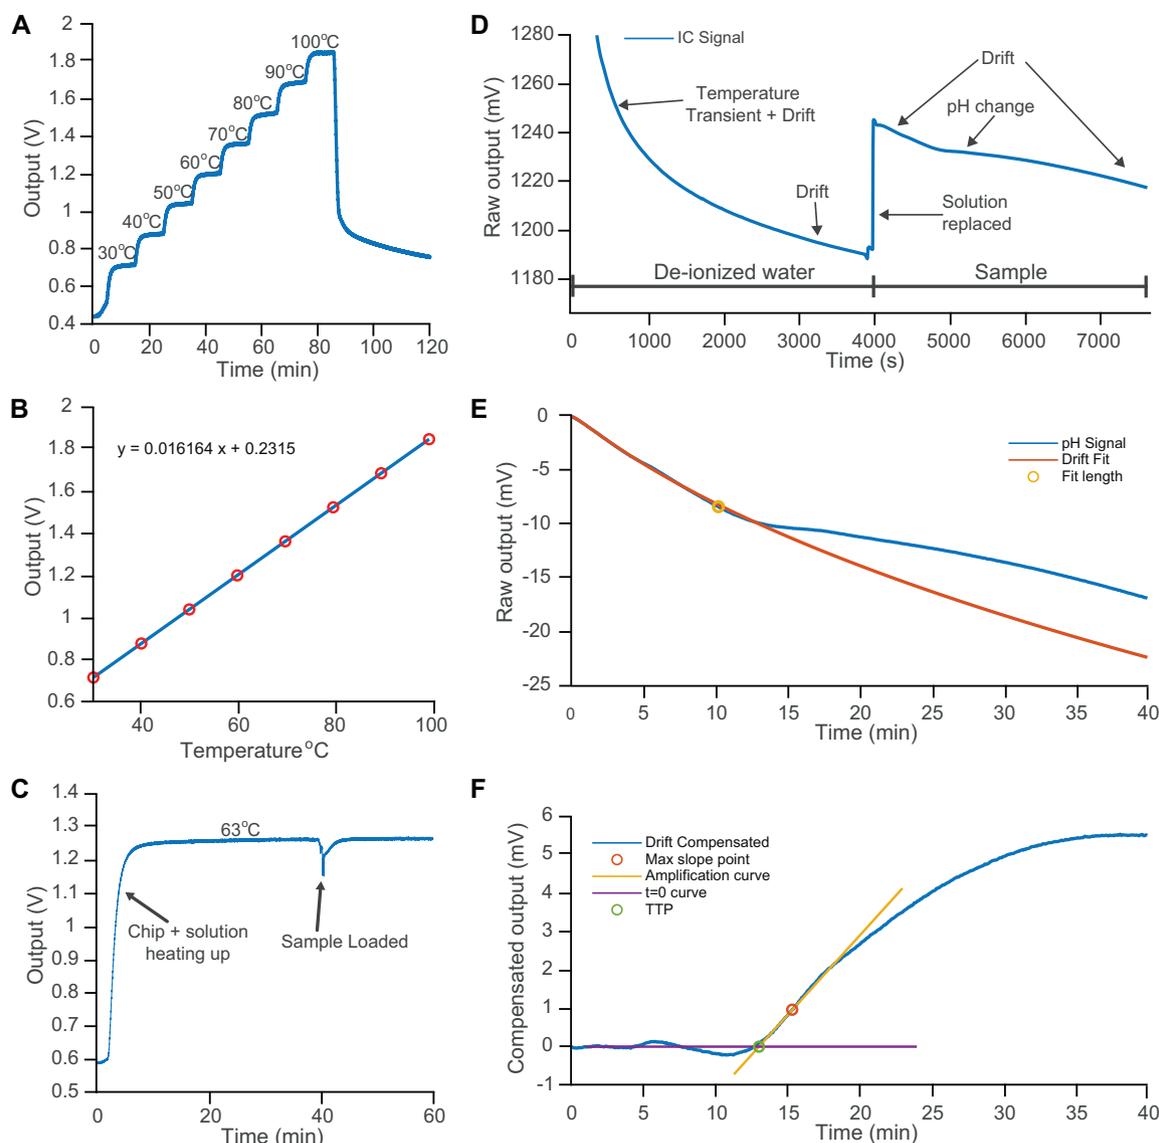


Fig. 2. Temperature Sensor and Data Processing. (A) Temporal characterisation of the temperature sensor on-chip at steps of 10°C. (B) Temperature sensor linearity showing a sensitivity of 16.2 mV/°C. (C) Temperature profile from the on-chip sensor during a typical reaction. (D) Typical response obtained during a positive pH-LAMP carried-out in the LoC platform. The trace shows raw data recorded as the average of active pixels in the ISFET array. At first, the chip heats up with de-ionized water loaded in the chamber and a temperature transient is observed. Subsequently, the slow monotonic change shown corresponds to drift due to hydration of the sensing material. After the temperature has settled, the solution is replaced with a positive sample which induces a pH change. (E) Signal recorded from the ISFET sensors after the sample has been loaded. The stretched-exponential drift model is adopted whose parameters are fitted using temporal data from the first few (<10) minutes of the reaction. Subsequently, drift is extrapolated until the end of the amplification reaction and is assumed as the background signal. (F) Drift-compensated signal with the TTP obtained by finding the point where the amplification curve crosses $y = 0$. The amplification curve is obtained as the straight line at the point of maximum slope of the drift-compensated signal.

was recovered for further analysis.


DNA amplification modifies the overall pH of the loaded solution causing a proportional electronic (voltage) change sensed by the ISFETs, illustrated in Fig. 1D. When no amplification takes place, the pH of the solution remains the same leading to a constant voltage signal. Measurements of pH with a commercial pH meter line (Sentron SI600) and DNA quantification with a fluorometer (Qubit 3.0, Thermo Fisher Scientific) were obtained from the recovered solution to confirm whether amplification had occurred as well as the corresponding pH change.

Furthermore, a temperature sensor has been included on the microchip to monitor the temperature during DNA amplification reactions. The sensor is based on a typical PTAT circuit configuration with a linear response. Characterisation of the temperature sensor across a temperature range of 30–100°C is shown in Fig. 2A–B and the response

during a typical reaction in Fig. 2C.

2.3. Mechanism of pH-LAMP detection using ISFETs

During nucleic acid amplification, nucleotides are incorporated by action of a polymerase resulting in the release of a proton (H^+) as described in Eq. (2). The release of protons into the solution induces a change in pH that ISFETs can transduce into an electrical output, thus correlating a change in pH to a change in voltage (Toumazou et al., 2013).



where DNA_n indicates the n^{th} nucleotide and PPi is pyrophosphate. Additionally, this change is regulated by the buffer capacity (β_{int}) of the solution. Overall, the change in pH is given by:

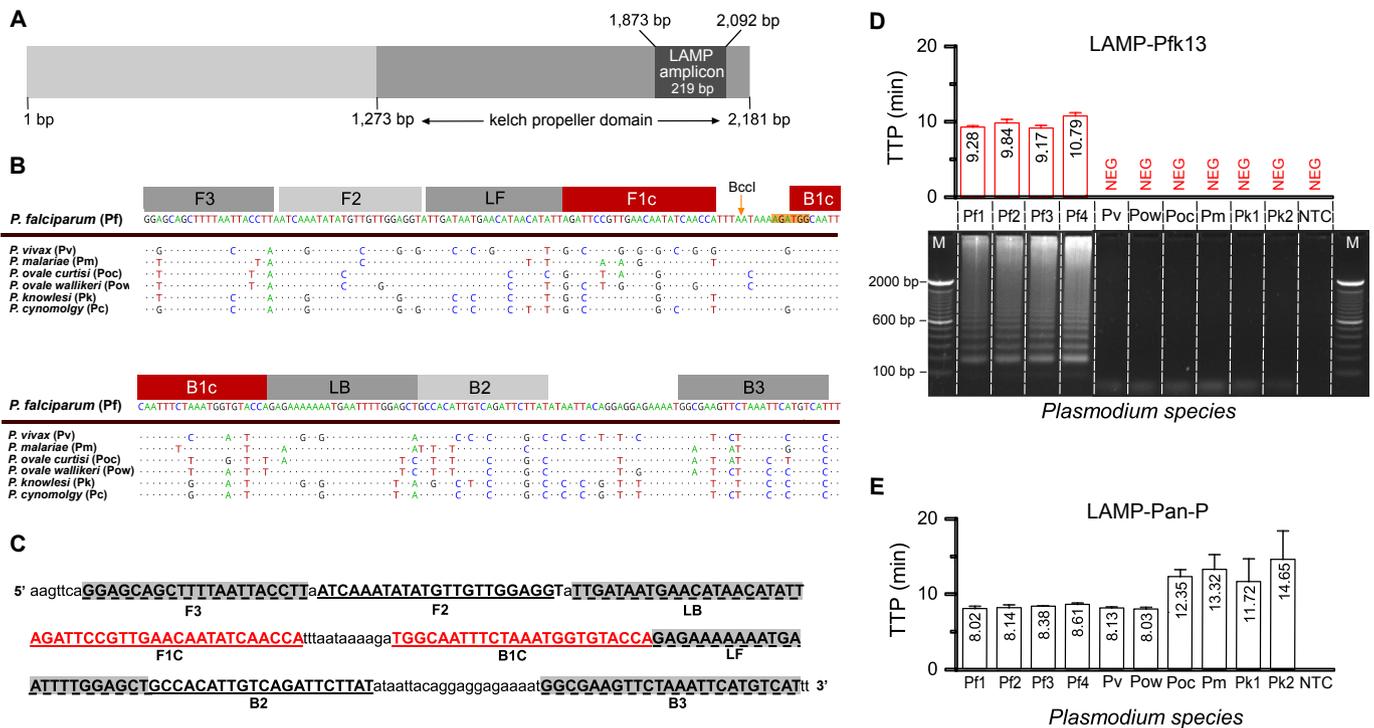


Fig. 3. Sequence alignment, designed primers and analytical specificity for the detection of *P. falciparum*. (A) Illustration of the gene *kelch 13* highlighting the location of the LAMP-PFK13 amplicon. (B) Alignment of all human-infective *Plasmodium* species with *P. falciparum* as the reference sequence. Mismatches in the alignment are displayed as AGTC whereas matched nucleotides are represented as dots. The LAMP-Pfk13 primers are illustrated on top of the alignment. (C) Primer location in LAMP amplicon (5' to 3' direction). Sequences of the primers can be found in Table S1. (D) Results showing specific amplification of *P. falciparum* DNA samples from clinical isolates as well as gel electrophoresis of the amplified products to confirm specificity. Digested amplification products are shown in Fig. S2. The restriction enzyme used for this experiment is BclI (#R0704S, New England BioLabs). The cutting point is illustrated with an arrow and the binding region is orange shadowed in (B). M denotes 100 bp DNA ladder (#10488058, Invitrogen). Acronyms are described in (B). (E) LAMP pan-primer set (Han et al., 2007) used as control for the detection of all *Plasmodium* species. TTP values are displayed in minutes and labelled. (For interpretation of the references to color in this figure legend, the reader is referred to the Web version of this article.)

$$\Delta pH = N \frac{H^+}{\beta_{int}} \quad (3)$$

where N denotes the total number of nucleotides incorporated during amplification. Consequently, the pH change is proportional to the total number of nucleotides inserted and inversely proportional to the buffering capacity of the solution. As a result, this opens up the possibility of electronic sensing, whereby ISFETs can be used to track the pH change during nucleic acid amplification. The expected modification in ISFETs is described by modifying Eq. (1) to:

$$\Delta V_{chem} = \gamma + 2.3 \alpha U_T N \frac{H^+}{\beta_{int}} \quad (4)$$

This equation can be used to describe the amplification curve which follows an exponential profile. At the early stages of the reaction, the amount of protons generated is not enough to overcome the buffering capacity of the solution and could also be very small compared to the sensitivity of the sensing layer. Eventually, the amount of protons accumulated is enough for showing a detectable (exponential) signal. Subsequently, as the amount of reagents is exhausted, the reaction profile enters the saturation stage and reaches a plateau.

2.4. Data analysis

During an amplification reaction, the pH signal is obtained by taking the average of the active sensors that are exposed to the solution. The signal includes drift due to the hydration of Si_3N_4 used for sensing which manifests as a slow, monotonic change on the output (Jamasp, 2004). The underlying cause is the diffusion of ions from the solution to charge-trapping sites in the nitride that exist due to its amorphous

structure. This phenomenon can be modelled as a dispersive transport process following a stretched-exponential response ($\exp[-t^\beta]$). Consequently, the first few minutes (<10) of the amplification reaction are used to sample drift and derive an analytical equation that fits the drift observed. As a result, the pH signal can be decoupled from the expected drift and the pH change due to DNA amplification can be obtained. To ensure accurate modelling of drift, the compensation method is applied locally around the exponential amplification point and is not considered valid at large extrapolated values of the drift model. Responses before and after drift compensation are shown in Fig. 2D–F.

Furthermore, after obtaining the drift-compensated signal which captures the pH change due to amplification, the time-to-positive (TTP) metric is obtained. To improve the robustness of extracting TTP in the case of sub-optimal amplification conditions, an alternative metric to C_t , called C_y , has been considered. This metric has been shown to be more reliable than C_t when considering samples of different efficiencies and is described by the intersection point between the time axis (or cycles) and the tangent of the inflection point of the amplification response (Guescini et al., 2008; Subramanian and Gomez, 2014). For comparison, both C_y and C_t values have been derived from the fluorescent data obtained earlier with the LC96 instrument, and we show that they are perfectly correlated i.e. following a linear and monotonic relationship. The specific data considered are included in Table S2. As a result, the C_y metric is also suitable for quantification purposes and has been used here when considering LoC data which do not rely on fluorescent measurements. The combination of these two methods (drift compensation and C_y) is outlined below and illustrated graphically in Fig. 2. Bold notation (e.g. \mathbf{v}) is used to indicate vectors or time series.

1. The pH signal \mathbf{p} obtained from an amplification reaction is

- normalized by removing the DC component (background).
- During the first few minutes (<10) after the sample is loaded, sensor drift is modelled using $\mathbf{d} = \exp\left[\alpha - \left(\frac{t}{\tau}\right)^\beta\right]$ where the scalar parameters α , τ and β are estimated.
 - \mathbf{d} is extrapolated until the completion of the amplification reaction.
 - The drift-compensated response is obtained using $\mathbf{p} - \mathbf{d}$.
 - The inflection point is determined as the point of maximum derivative of $\mathbf{p} - \mathbf{d}$. A linear response is fitted around the maximum derivative point (amplification curve).
 - TTP is defined as the time when the amplification curve crosses $y = 0$.

Results obtained with the LoC platform prior to any processing steps are shown in Fig. S4.

3. Results

3.1. Analytical specificity of the *P. falciparum* LAMP assay

The selected region of the kelch propeller domain within the gene *kelch 13* for *P. falciparum* specific detection is shown in Fig. 3A. Alignment of consensus sequences of all human-infective *Plasmodium* species is presented in Fig. 3B, with the location of the 6 primers in Fig. 3C.

To illustrate the LAMP-Pfk13 primer specificity, gDNA samples from several human-infective *Plasmodium* species (*P. falciparum*, *P. malariae*, *P. vivax*, *P. ovale curtisi*, *P. ovale wallikeri* and *P. knowlesi*) were tested using a commercial LC96 qPCR instrument. This sample set included two additional *P. falciparum* samples with mutations related to artemisinin-resistance (Pf3 which carries the mutation C580Y, and sample Pf4 which harbours the mutation Y493H). Fig. 3D shows the time-to-positive (TTP) values obtained from the LAMP reactions which specifically detected the *P. falciparum* samples (Pf1, Pf2, Pf3 and Pf4). To further confirm specificity, a gel electrophoresis containing the post-amplification products is shown in Fig. 3D. Digested amplified products with the restriction enzyme BclI (#R0704S, New England Biolabs) are shown in Fig. S2. These results demonstrate the absence of cross-reactivity across the *Plasmodium* species with the designed primer set LAMP-Pfk13. As a control, Fig. 3E shows the time-to-positive (TTP) values obtained from the amplification reactions with a Pan-*Plasmodium* LAMP primer set (Han et al., 2007) which is able to detect all species.

Prior to this study, only one PCR primer set was reported targeting the gene *kelch 13* (Talundzic et al., 2015) yet without being accompanied by any information regarding the limit of detection. To the best of our knowledge, this is the first isothermal assay targeting the gene *kelch 13* with high specificity for *P. falciparum* identification.

3.2. Analytical sensitivity of *P. falciparum* LAMP assay

The novel LAMP assay, LAMP-Pfk13, was tested in the LC96 instrument with ten-fold serial dilutions of *P. falciparum* synthetic DNA ran in triplicates, ranging from 10^7 to 1 copies per reaction. The standard curve generated from these results is shown in Fig. 4A with high linearity ($R^2 = 0.993$), a limit of detection of 1 copy per reaction and TTP values ranging from 6 to 19 min. The amplification curves are included in Fig. S3 and the TTP values were obtained using the cycle-threshold metric, C_t , set at 0.2 normalized fluorescence units by the LC96 instrument. Based on the results obtained, rapid quantification of unknown samples is possible with high reliability.

Furthermore, the performance of pH-LAMP was evaluated by adjusting the buffering capabilities as described in Section 2.1.2. The corresponding amplification curves of pH-LAMP are shown in Fig. S3 and the standard curve in Fig. 4A. In this case, the limit of detection achieved was 10 copies per reaction with an associated $R^2 = 0.991$ and

TTP values ranging from 9 to 22 min.

To illustrate and compare the two metrics considered for TTP estimation, both C_y and C_t values have been derived from the raw fluorescent data obtained using the LC96 instrument. The specific data considered are included in Table S2 and we show that they are perfectly correlated, i.e. following a linear and monotonic relationship. Therefore both could be used to build a standard curve for quantification purposes.

3.3. CMOS-based Lab-on-Chip detection and quantification of *P. falciparum*

Based on the previous results, the designed primer set enables specific, sensitive and rapid detection of *P. falciparum*. Consequently, this section describes the results obtained by conducting the pH-LAMP amplification reactions on the Lab-on-Chip platform shown in Fig. 1C.

Several concentrations of *P. falciparum* synthetic DNA (10^7 , 10^5 and 10^3 copies per reaction) were tested in duplicates in the LoC platform to evaluate its capability for nucleic acid amplification and quantification. Amplification responses from carrying-out pH-LAMP, in the form of pH-to-voltage signals, were post-processed in software to compensate for known ISFET non-idealities such as sensor drift and thus obtain (i) average and normalized amplification curves and (ii) TTP values using the C_y method. The standard curve built with LoC data and used for quantification is shown in Fig. 4A, with the LoC amplification curves in Fig. 4B. In comparison, Fig. 4C shows the respective responses from the LC96 instrument used as reference. The TTP values obtained across the various DNA concentrations from both the LoC and LC96 are illustrated and compared in Fig. 4D. Statistical analysis of these results using Student's t-test to compare means as well as correlation test to compare trends, report a p-value <0.0001 and a correlation coefficient of 0.99 (more details in Table S3). These metrics indicate that there exists an insignificant probability of unequal concentrations producing similar TTP values and that the trends across concentrations are almost perfectly dependent. Overall, the robustness of the LoC against a commercial instrument is demonstrated for DNA quantification which is consistent with the standard curves presented earlier in Fig. 4A.

To further confirm LoC amplification, the pH of the solution was measured before and after incubation at 63°C using a commercial (Sentron SI600) pH meter. Specifically, Fig. 4E shows the Δ pH obtained from running reactions at the same DNA concentration in the LC96 instrument as well as in the LoC. pH measurements and DNA quantification values can be found in Tables S4 and S5. In addition, the figure includes the equivalent pH obtained from the output of the ISFET sensors with the previously determined sensitivity of 9.23 mV/pH. A small pH change due to slight increased DNA concentration was observed for non-template control samples. Nevertheless a wide error margin was obtained which can be used to set a pH threshold indicating amplification through the recorded pH change.

To demonstrate the quantification capabilities of unknown samples, two *P. falciparum* gDNA samples derived from clinical isolates were amplified and quantified using both the LoC and reference LC96 instrument. Representative amplification curves obtained from both reactions as well as negative control are shown in Fig. 4F–G. Furthermore, Fig. 4H shows the quantification of the unknown samples from duplicate reactions using the previously derived standard curves. The estimated initial genomic concentration values obtained with the LoC are within < 10% from the reference demonstrating the capability of the LoC to quantify clinical isolates accurately.⁴

⁴ The percentage change was calculated by referring the concentration values (i.e. 10^x) to a linear axis.

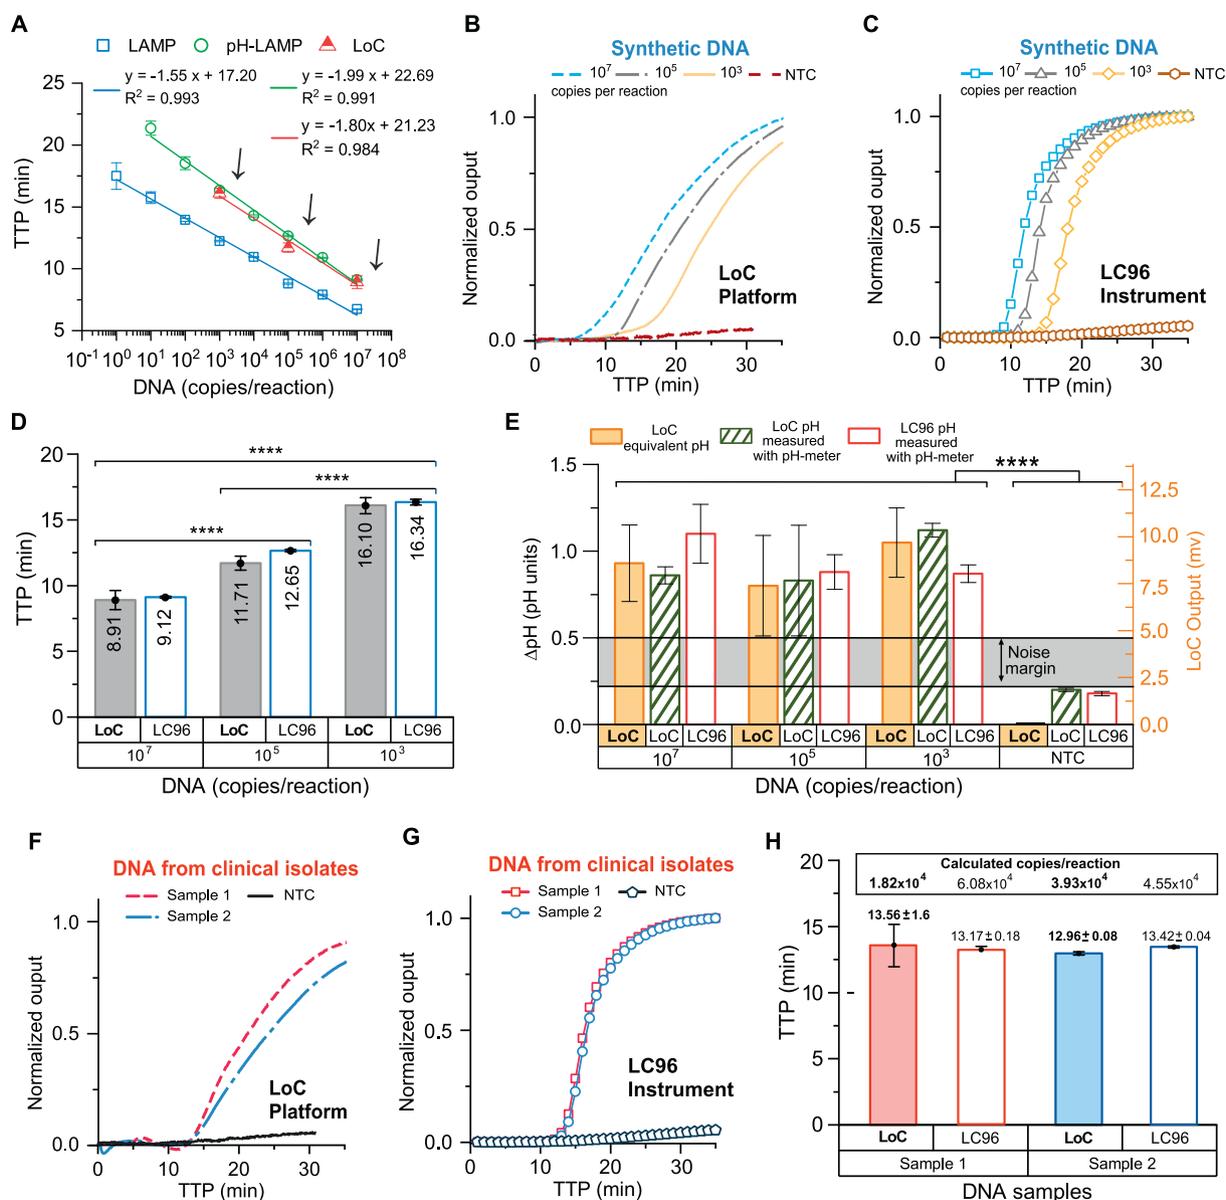


Fig. 4. Summary of results of *P. falciparum* amplification with the LoC platform and a commercial qPCR instrument. (A) LAMP, pH-LAMP and LoC pH-LAMP standard curves obtained with the primer set LAMP-PfK13. Both pH-LAMP and the LoC curves are almost perfectly correlated to the LAMP reference. **(B)** Amplification curves of synthetic DNA at different concentrations (10^7 , 10^5 and 10^3 copies per reaction) carried-out in the LoC platform ($n = 2$). **(C)** Same samples carried out in LC96 qPCR instrument ($n = 3$). **(D)** Bar plot comparing the TTP values obtained with the LoC platform and the LC96 qPCR instrument at the different concentrations of synthetic DNA. P-values produced from the Student's t-test are shown as stars, with **** representing p-value < 0.0001. **(E)** Bar plot showing Δ pH measurements of the reaction solutions obtained before and after incubation at 63°C with the LoC (green striped bars) and the LC96 qPCR instrument (white bars with red edges). Furthermore, the LoC signal output (yellow bars) is shown in mV (right-hand side Y-axis) and equivalent pH units according to the sensitivity described in Section 2.2 (left-hand side Y-axis). **(F)** Representative example of amplification curves of two *P. falciparum* DNA samples derived from clinical isolates and a negative control, carried-out in the LoC platform. **(G)** Same samples carried-out in the LC96 qPCR instrument. **(H)** Bar plot comparing the TTP values of detecting clinical isolates, such as the ones shown in F and G, for quantification purposes. Also annotated are the equivalent concentrations estimated using the LoC and pH-LAMP standard curves in (A). (For interpretation of the references to color in this figure legend, the reader is referred to the Web version of this article.)

3.4. CMOS-based Lab-on-Chip detection of *P. falciparum* drug-resistant malaria

The most common mutation indicating the presence of drug-resistant parasites is the C580Y single nucleotide polymorphism (SNP). The LAMP-based method described in Malpartida-Cardenas et al. (2018) reported the discrimination of wild-type (WT) from mutant (MT) alleles by robustly preventing or delaying unspecific amplification, as illustrated in Fig. 5A. Two reactions are tested, one targeting the presence of the WT allele (WT reaction) and another one targeting the presence of the MT allele (MT reaction). Primer sequences can be found

in Table S6. In this case, this method was adapted to pH-LAMP in order to be transferred onto the Lab-on-Chip platform.

P. falciparum DNA samples from clinical isolates known to be WT or MT were tested with the LoC platform and with the LC96 qPCR instrument as control. Results are presented in Fig. 5B, showing the TTP values obtained with each reaction. Overall, SNP discrimination is possible due to delayed amplification of unspecific targets leading to a difference in TTP values (Δ TTP). As a result, the capability of the LoC platform to discriminate alleles is illustrated in the same way as the commercial LC96 qPCR instrument.

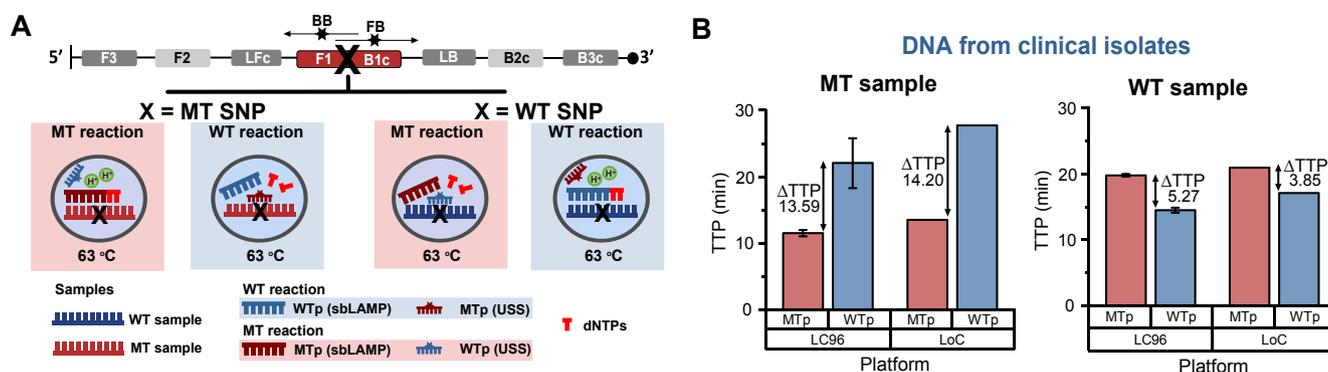


Fig. 5. Lab-on-Chip detection of *C580Y* SNP associated to *P. falciparum* artemisinin-resistance. (A) Schematic representation of the USS-sbLAMP method for allele-specific detection (Malpartida-Cardenas et al., 2018). Specific reactions amplify in isothermal conditions whereas unspecific reactions are prevented or delayed. (B) Comparison of results obtained with the LoC platform and the LC96 qPCR instrument. TTP values are displayed in minutes, with Δ TTP values annotated, indicating that specific reactions always occur earlier. MTp = mutant primer set; WTP = wild type primer set.

4. Discussion

Our results demonstrate that the developed LAMP assays paired to the LoC platform are well-suited for clinical applications with significant potential towards point-of-care implementations. This is achieved by tailoring amplification chemistries to be compatible with electronic detection using an ISFET-based platform and a Lab-on-Chip approach. We demonstrate the potential of such an implementation for the detection of malaria-causing *P. falciparum* using a novel and specific primer set as well as specific identification of drug-resistant mutations. Furthermore, we show for the first time *P. falciparum* DNA quantification on a LoC platform with high accuracy and robustness comparable with a commercial benchtop instrument.

Compared to other rapid diagnostic tests for pathogen detection, we opted for nucleic-acid-based due to their high sensitivity and specificity. Even though PCR is considered the gold standard, in this case isothermal amplification using LAMP avoids the need for complex temperature control, is more specific and rapid and is therefore more suited for point-of-care applications. Furthermore, there is no need for pre-treatment at different temperatures for optimal DNA amplification (Walker et al., 1992). Results obtained with the LAMP assay targeting the gene *kelch 13* in *P. falciparum* show high specificity without cross-reactivity across other *Plasmodium* species and high sensitivity with a limit of detection of 1 copy per reaction. In contrast to prior works which target the gene 18S rRNA (Mohon et al., 2014; Lau et al., 2016; Han et al., 2007; Poon et al., 2006), the gene *kelch 13* does not present highly inter-species conserved regions thus ensuring higher specificity, and the speed of detection shown here is less than 20 min. In addition, modifying the reaction chemistries to pH-LAMP for electrochemical compatibility is achieved with almost identical behaviour, indicating the feasibility of carrying-out the reactions in an ISFET-based platform.

The developed LoC platform leverages on ISFET-based detection to facilitate fully-electronic chemical sensing and direct electrochemical signal transduction (Miscourides and Georgiou, 2019). Sensor fabrication in CMOS technology achieves sensor miniaturisation, low cost manufacturing, scalability and sensitivity which are necessary for a point-of-care implementation. Furthermore, detection takes place with sensors fabricated in unmodified CMOS technology without the use of probes, electrodes or prior surface treatment. LoC detection has been demonstrated for DNA amplification reactions with results matching those from a commercial benchtop instrument and allowing for building the first LoC standard curve.

Slight deviations between the TTP values obtained with the LoC platform and the LC96 instrument could be attributed to several factors such as (i) intrinsic error among technical replicates, (ii) reaction conditions variability such as different material of the reaction chamber, (iii) chip non-idealities such as trapped charge or variations in

the sensing Si_3N_4 layer, and (iv) the different nature of the detected signal (pH-vs-fluorescence). Specifically, fluorescence measurements are obtained as the intercalating dye is being incorporated in newly generated amplicons (Biebricher et al., 2015; Eischeid, 2011; Hannah and Armitage, 2004). On the contrary, in the LoC platform the chemical input in the form of $[H^+]$ concentration ($pH = -\log[H^+]$) is converted to an electrical output. Multiple amplification events take place simultaneously in LAMP, and therefore, describing the kinetics of this assay is not trivial as well as establishing a relationship between fluorescence and change in pH (Subramanian and Gomez, 2014; Sun et al., 2014; Khoshosheva et al., 2016). Nevertheless, the high degree of correlation recorded between the TTP values obtained using both types of responses implies that both can be used as indicators of the amplification state, something that was previously argued in (Toumazou et al., 2013). The standard curve was validated with unknown DNA samples from clinical isolates with high accuracy, demonstrating the feasibility of DNA quantification on-chip. In addition, SNP discrimination on the LoC platform was achieved with DNA samples harbouring the *C580Y* mutation derived from clinical isolates.

Nevertheless, to fully realize a PoC platform for *P. falciparum* and drug-resistant malaria detection, several issues need to be optimised further. Firstly, the current workflow still relies on the use of extracted DNA rather than samples directly obtained from patients (e.g. from bodily fluids most typically blood). Consequently, the introduction of a sample preparation step is necessary in order for such an approach to be fully deployed as Point-of-Care sample-to-result platform. Nevertheless, isothermal techniques and specifically LAMP which was employed here, has been shown to be more robust to typical blood inhibitors compared to PCR (Poon et al., 2006) which can be leveraged to simplify such a sample preparation process. Secondly, from an electronic aspect, embedded temperature control is key for achieving full portability since temperature in the LoC platform presented here is controlled using an external instrument. That extends to enclosing all electronic functions into portable packaging with embedded temperature control, isolating the microchip and microfluidic modules in the form of a disposable cartridge from the base unit responsible for data readout and processing. Towards this direction, we have already designed a reusable motherboard and a disposable cartridge module. The cartridge only includes the sensing microchip, microfluidic setup and amplification reagents while leveraging on CMOS technology to ensure mass manufacture of sensors and thus low-cost, suitable for point-of-care applications.

5. Conclusion

In this paper, we show rapid and specific diagnosis of *P. falciparum* malaria as well as the identification of mutations related to drug-

resistance using both a commercial qPCR instrument and a custom Lab-on-Chip Platform. The performance of the LoC platform was comparable with the commercial instrument and has been used for derivation of the first LoC standard curve and consequently, the quantification of unknown samples. Taking into consideration the advantages of using LAMP, we anticipate that using the LoC platform without a complex sample preparation step, will further reduce the cost maintaining the time-to-results. Leveraging on the speed of detection, specificity and sensitivity achieved with the LoC platform, we expect to further validate this platform in resource-limited settings towards the rapid diagnosis of infectious diseases at the point-of-care, epidemiological surveillance and reduction of antimicrobial resistance.

Declaration of interest

None.

CRediT authorship contribution statement

Kenny Malpartida-Cardenas: Investigation, Data curation, Formal analysis, Methodology, Writing - original draft, Writing - review & editing. **Nicholas Miscourides:** Investigation, Data curation, Formal analysis, Methodology, Writing - original draft, Writing - review & editing. **Jesus Rodriguez-Manzano:** Supervision, Conceptualization, Funding acquisition, Methodology, Writing - original draft, Writing - review & editing. **Ling-Shan Yu:** Methodology, Writing - review & editing. **Nicolas Moser:** Methodology, Writing - review & editing. **Jake Baum:** Conceptualization, Funding acquisition, Writing - review & editing. **Pantelis Georgiou:** Supervision, Conceptualization, Funding acquisition, Writing - review & editing.

Declaration of competing interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Acknowledgements

This work was supported by the EPSRC HiPEDS Centre for Doctoral Training [EP/L016796/1 to K.M.C. and N.M.]. We would like to acknowledge the Imperial Confidence in Concepts - Joint Translational Fund (PS3111EESA to P.G. and J.R.M.); the EPSRC Pathways to Impact (PSE394EESA to P.G. and J.R.M.); the EPSRC Global Challenge Research Fund [EP/P510798/1 to P.G., J.B., and J.R.M.]; the Wellcome Investigator Award [100993/Z/13/Z to J.B.] and the Medical Research Council (MRC) (Newton Fund award to J.B. [MR/N012275/1]).

Appendix A. Supplementary data

Supplementary data to this article can be found online at <https://doi.org/10.1016/j.bios.2019.111678>.

References

Aurrecochea, C., Brestelli, J., Brunk, B.P., Dommer, J., Fischer, S., Gajria, B., Gao, X., Gingle, A., Grant, G., Harb, O.S., Heiges, M., Innamorato, F., Iodice, J., Kissinger, J.C., Kraemer, E., Li, W., Miller, J.A., Nayak, V., Pennington, C., Pinney, D.F., Roos, D.S., Ross, C., Stoeckert, C.J., Treatman, C., Wang, H., 2009. PlasmoDB: a functional genomic database for malaria parasites. *Nucleic Acids Res.* 37, D539–D543.

Banoth, E., Kasula, V.K., Jagannadh, V.K., Gorthi, S.S., 2016. Optofluidic single-cell absorption flow analyzer for point-of-care diagnosis of malaria. *J. Biophot.* 9, 610–618.

Beshir, K.B., Sepúlveda, N., Bharmal, J., Robinson, A., Mwanguzi, J., Busula, A.O., de Boer, J.G., Sutherland, C., Cunningham, J., Hopkins, H., 2017. *Plasmodium falciparum* parasites with histidine-rich protein 2 (pfrp2) and pfrp3 gene deletions in two endemic regions of Kenya. *Sci. Rep.* 7, 14718.

Biebricher, A.S., Heller, I., Roijmans, R.F.H., Hoekstra, T.P., Peterman, E.J.G., Wuite, G.J.L., 2015. The impact of DNA intercalators on DNA and DNA-processing enzymes elucidated through force-dependent binding kinetics. *Nat. Commun.* 6, 7304.

Bronner, U., Divis, P.C., Farnert, A., Singh, B., 2009. Swedish traveller with Plasmodium knowlesi malaria after visiting Malaysian Borneo: a case report. *Malar. J.* 8, 15.

Cacho-Soblechero, M., Malpartida-Cardenas, K., Moser, N., Georgiou, P., 2019. Programmable ion-sensing using oscillator-based isfet architectures. *IEEE Sens. J.* 19 (19), 8563–8575.

Cheng, Q., Gattton, M.L., Barnwell, J., Chiodini, P., McCarthy, J., Bell, D., Cunningham, J., 2014. *Plasmodium falciparum* parasites lacking histidine-rich protein 2 and 3: a review and recommendations for accurate reporting. *Malar. J.* 13, 283.

Edgar, R.C., 2004. MUSCLE: multiple sequence alignment with high accuracy and high throughput. *Nucleic Acids Res.* 32, 1792–1797.

Eisheid, A.C., 2011. SYTO dyes and EvaGreen outperform SYBR Green in real-time PCR. *BMC Res. Notes* 4, 263.

Georgiou, P., Toumazou, C., 2009. ISFET characteristics in CMOS and their application to weak inversion operation. *Sens. Actuators B Chem.* 143, 211–217.

Guescini, M., Sisti, D., Rocchi, M., Stocchi, L., Stocchi, V., 2008. A new real-time PCR method to overcome significant quantitative inaccuracy due to slight amplification inhibition. *BMC Bioinf.* 9, 326–337.

Han, E.-T., Watanabe, R., Sattabongkot, J., Khuntirat, B., Sirichaisinthop, J., Iriko, H., Jin, L., Takeo, S., Tsuboi, T., 2007. Detection of four plasmodium species by genus- and species-specific loop-mediated isothermal amplification for clinical diagnosis. *J. Clin. Microbiol.* 45, 2521–2528.

Hannah, K.C., Armitage, B.A., 2004. DNA-templated assembly of helical cyanine dye aggregates: a supramolecular chain polymerization. *Acc. Chem. Res.* 37, 845–853.

Hou, H.W., Bhagat, A.A.S., Lin Chong, A.G., Mao, P., Wei Tan, K.S., Han, J., Lim, C.T., 2010. Deformability based cell margination—A simple microfluidic design for malaria-infected erythrocyte separation. *Lab Chip* 10, 2605.

Hu, J., Wang, S., Wang, L., Li, F., Pinguan-Murphy, B., Lu, T.J., Xu, F., 2014. Advances in paper-based point-of-care diagnostics. *Biosens. Bioelectron.* 54, 585–597.

Jamasb, S., 2004. An analytical technique for countering drift in ion-selective field effect transistors (ISFETs). *IEEE Sens. J.* 4, 795–801.

Kearse, M., Moir, R., Wilson, A., Stones-Havas, S., Cheung, M., Sturrock, S., Buxton, S., Cooper, A., Markowitz, S., Duran, C., Thierer, T., Ashton, B., Meintjes, P., Drummond, A., 2012. Geneious Basic: an integrated and extendable desktop software platform for the organization and analysis of sequence data. *Bioinformatics* 28, 1647–1649.

Khan, M., Khan, A.R., Shin, J.H., Park, S.Y., 2016. A liquid-crystal-based DNA biosensor for pathogen detection. *Sci. Rep.* 6, 1–11.

Khorosheva, E.M., Karymov, M.A., Selck, D.A., Ismagilov, R.F., 2016. Lack of correlation between reaction speed and analytical sensitivity in isothermal amplification reveals the value of digital methods for optimization: validation using digital real-time RT-LAMP. *Nucleic Acids Res.* 44 e10–e10.

Kozel, T.R., Burnham-Marusch, A.R., 2017. Point-of-Care testing for infectious diseases: past, present, and future. *J. Clin. Microbiol.* 55, 2313–2320.

Krampa, F., Aniwah, Y., Awandare, G., Kanyong, P., 2017. Recent progress in the development of diagnostic tests for malaria. *Diagnostics* 7, 54.

Kurbanoglu, S., Dogan-Topal, B., Rodriguez, E.P., Bozal-Palabiyik, B., Ozkan, S.A., Uslu, B., 2016. Advances in electrochemical DNA biosensors and their interaction mechanism with pharmaceuticals. *J. Electroanal. Chem.* 775, 8–26.

Labuda, J., Brett, A.M.O., Evtugyn, G., Fojta, M., Mascini, M., Osoz, M., Palchetti, I., Paleček, E., Wang, J., 2010. Electrochemical nucleic acid-based biosensors: Concepts, terms, and methodology (IUPAC Technical Report). *Pure Appl. Chem.* 82.

Lau, Y.-L., Lai, M.-Y., Fong, M.-Y., Jelip, J., Mahmud, R., 2016. Loop-mediated isothermal amplification assay for identification of five human plasmodium species in Malaysia. *Am. J. Trop. Med. Hyg.* 94, 336–339.

Law, Y.-H., 2018. Rare human outbreak of monkey malaria detected in Malaysia. *Nature*.

Lee, H., Sun, E., Ham, D., Weissleder, R., 2008. Chip-NMR biosensor for detection and molecular analysis of cells. *Nat. Med.* 14, 869–874.

Liu, X., Peaslee, D., Jost, C.Z., Baumann, T.F., Majzoub, E.H., 2011. Systematic pore-size effects of nanoconfinement of LiBH₄: elimination of diborane release and tunable behavior for hydrogen storage applications. *Chem. Mater.* 23, 1331–1336.

Malpartida-Cardenas, K., Rodriguez-Manzano, J., Yu, L.-S., Delves, M.J., Nguon, C., Chotivanich, K., Baum, J., Georgiou, P., 2018. Allele-specific isothermal amplification method using unmodified self-stabilizing competitive primers. *Anal. Chem.* 90, 11972–11980.

Mangold, M., Manson, K., Koay, S., Stephens, R., Thomson, P., Peterson, K., 2005. Real-time PCR for detection and identification of *Plasmodium* spp.. *J. Clin. Microbiol.* 43, 2435–2440.

Miscourides, N., Georgiou, P., 2019. ISFET arrays in CMOS: a head-to-head comparison between voltage and current mode. *IEEE Sens. J.* 19, 1224–1238.

Miscourides, N., Yu, L.-S., Rodriguez-Manzano, J., Georgiou, P., 2018. A 12.8 k current-mode velocity-saturation ISFET array for on-chip real-time DNA detection. *IEEE Trans. Biomed. Circuits Syst.* 1–13.

Mohon, A.N., Elahi, R., Khan, W.A., Haque, R., Sullivan, D.J., Alam, M.S., 2014. A new visually improved and sensitive loop mediated isothermal amplification (LAMP) for diagnosis of symptomatic falciparum malaria. *Acta Trop.* 134, 52–57.

Moody, A., 2002. Rapid diagnostic tests for malaria parasites. *Clin. Microbiol. Rev.* 15, 66–78.

Moon, R.W., Hall, J., Rangkuti, F., Ho, Y.S., Almond, N., Mitchell, G.H., Pain, A., Holder, A.A., Blackman, M.J., 2013. Adaptation of the genetically tractable malaria pathogen *Plasmodium knowlesi* to continuous culture in human erythrocytes. *Proc. Natl. Acad. Sci.* 110, 531–536.

Moser, N., Rodriguez-Manzano, J., Lande, T.S., Georgiou, P., 2018. A scalable ISFET sensing and memory array with sensor auto-calibration for on-chip real-time DNA detection. *IEEE Trans. Biomed. Circuits Syst.* 1–12.

Notomi, T., Okayama, H., Masubuchi, H., Yonekawa, T., Watanabe, K., Amino, N., Hase, T., 2000. Loop-mediated isothermal amplification of DNA. *Nucleic Acids Res.* 28, E63.

- Obahiagbon, U., Smith, J.T., Zhu, M., Katchman, B.A., Arafa, H., Anderson, K.S., Blain Christen, J.M., 2018. A compact, low-cost, quantitative and multiplexed fluorescence detection platform for point-of-care applications. *Biosens. Bioelectron.* 117, 153–160.
- Polley, S.D., Mori, Y., Watson, J., Perkins, M.D., González, I.J., Notomi, T., Chiodini, P.L., Sutherland, C.J., 2010. Mitochondrial DNA targets increase sensitivity of malaria detection using loop-mediated isothermal amplification. *J. Clin. Microbiol.* 48, 2866–2871.
- Poon, L.L.M., Wong, B.W.Y., Ma, E.H.T., Chan, K.H., Chow, L.M.C., Abeyewickreme, W., Tangpukdee, N., Yuen, K.Y., Guan, Y., Looareesuwan, S., Peiris, J.S.M., 2006. Sensitive and inexpensive molecular test for falciparum malaria: detecting plasmodium falciparum dna directly from heat-treated blood by loop-mediated isothermal amplification. *Clin. Chem.* 52, 303–306.
- Rodriguez-Manzano, J., Karymov, M.A., Begolo, S., Selck, D.A., Zhukov, D.V., Jue, E., Ismagilov, R.F., 2016. Reading out single-molecule digital RNA and DNA isothermal amplification in nanoliter volumes with unmodified camera phones. *ACS Nano* 10, 3102–3113.
- Singh, B., Bobogare, A., Cox-Singh, J., Snounou, G., Abdullah, M.S., Rahman, H.A., 1999. A genus- and species-specific nested polymerase chain reaction malaria detection assay for epidemiologic studies. *Am. J. Trop. Med. Hyg.* 60, 687–692.
- Subramanian, S., Gomez, R.D., 2014. An empirical approach for quantifying loop-mediated isothermal amplification (LAMP) using *Escherichia coli* as a model system. *PLoS One* 9, e100596.
- Sun, B., Rodriguez-Manzano, J., Selck, D.A., Khorosheva, E., Karymov, M.A., Ismagilov, R.F., 2014. Measuring fate and rate of single-molecule competition of amplification and restriction digestion, and its use for rapid genotype tested with hepatitis c viral rna. *Angew. Chem. Int. Ed.* 53, 8088–8092.
- Talundzic, E., Chenet, S.M., Goldman, I.F., Patel, D.S., Nelson, J.A., Plucinski, M.M., Barnwell, J.W., Udhayakumar, V., 2015. Genetic analysis and species specific amplification of the artemisinin resistance-associated kelch propeller domain in *P. falciparum* and *P. vivax*. *PLoS One* 10, e0136099.
- Toumazou, C., Shepherd, L.M., Reed, S.C., Chen, G.I., Patel, A., Garner, D.M., Wang, C.-J. a., Ou, C.-P., Amin-Desai, K., Athanasiou, P., Bai, H., Brizido, I.M.Q., Caldwell, B., Coomber-Alford, D., Georgiou, P., Jordan, K.S., Joyce, J.C., La Mura, M., Morley, D., Sathyavvruthan, S., Temelso, S., Thomas, R.E., Zhang, L., 2013. Simultaneous DNA amplification and detection using a pH-sensing semiconductor system. *Nat. Methods* 10, 641–646.
- Vashist, S., 2017. Point-of-Care diagnostics: recent advances and trends. *Biosensors* 7, 62.
- Walker, G.T., Fraiser, M.S., Schram, J.L., Little, M.C., Nadeau, J.G., Malinowski, D.P., 1992. Strand displacement amplification—an isothermal, in vitro DNA amplification technique. *Nucleic Acids Res.* 20, 1691–1696.
- Wong, Y.-P., Othman, S., Lau, Y.-L., Radu, S., Chee, H.-Y., 2018. Loop-mediated isothermal amplification (LAMP): a versatile technique for detection of microorganisms. *J. Appl. Microbiol.* 124, 626–643.
- Wongsrichanalai, C., Barcus, M.J., Muth, S., Sutamihardja, A., Wernsdorfer, W.H., 2007. A review of malaria diagnostic tools: microscopy and rapid diagnostic test (RDT). *Am. J. Trop. Med. Hyg.* 77, 119–127.
- World Health Organization (WHO), 2019. Fact Sheets: Infectious Diseases.
- Worldwide, H.D., 2019. Simple and Fast Malaria-LAMP Workflow.
- Yu, L.-S., Rodriguez-Manzano, J., Malpartida-Cardenas, K., Sewell, T., Bader, O., Armstrong-James, D., Fisher, M.C., Georgiou, P., 2019. Rapid and sensitive detection of azole-resistant *Aspergillus fumigatus* by tandem repeat loop-mediated isothermal amplification. *J. Mol. Diagn.* 21, 286–295.