

Original article

Low failure rate at short term for 40 mm heads and second generation triple annealed HCLPE liners in hybrid hip replacements

Rajkumar Thangaraj^{a,*}, Jan Kuiper^{b,c}, Ralph D. Perkins^a^a Princess Royal Hospital, Telford, United Kingdom^b ISTM, Keele University, Keele, ST5 5BG, United Kingdom^c Robert Jones and Agnes Hunt Orthopaedic Hospital NHS Foundation Trust, Oswestry, United Kingdom

ARTICLE INFO

Article history:

Received 24 October 2017

Received in revised form 19 December 2017

Accepted 21 December 2017

Available online 3 January 2018

Keywords:

Large diameter heads

Highly cross linked polyethylene

Sequentially processed polyethylene

Second generation HCLPE

Revision

Low failure

ABSTRACT

Introduction: 40 mm large diameter heads offer the advantages of lesser dislocation rates and better stability while highly cross linked polyethylene have lower wear rates than ultra high molecular weight polyethylene. Studies of the survivorship of 40 mm heads in hybrid hip replacements with Exeter stem and second generation highly cross linked polyethylene are limited. The purpose of the study is to report the short term of survivorship of the large diameter heads (40 mm) with Exeter stem with the secondary aim being the survival analysis of the thinnest second generation highly cross linked polyethylene.

Methods: Retrospective case series of survivorship of patients with hybrid hip replacements of Exeter stems with 40 mm heads articulating with second generation triple annealed highly cross linked polyethylene liner on a uncemented acetabular shell was performed. As a subset, survival of thinnest second generation highly cross linked polyethylene survival (3.8 mm) at short term was assessed. Survival of the implants was confirmed from the hospital records and National joint registry as of 2015. Revision for any cause was taken as end point.

Results: 324 hybrid hip replacements with 40 mm heads had been performed for primary hip osteoarthritis. Of the 324 hip replacements, 154 hip replacements had thinnest second generation highly cross linked polyethylene (3.8 mm). Two patients had revision of components, one for periprosthetic fracture and one for deep infection. Mean age of the patients was 70.5 years (range 42–88 years, median 71, SD 8.3 years). None of the patients had revision due to trunion wear or loosening of components. The overall 5-year implant survival probability of hips with 40 mm heads was 99.4% (95% CI 98 to 100%) while the subset group of hip replacements with thinnest second generation highly cross linked polyethylene (3.8 mm) had 5-year implant survival probability of 99.3% (95% CI 97.1 to 100%).

Conclusion: Short term survivorship does not show significant evidence of early failure or higher rate of revision in our series of hybrid hip replacements with large diameter heads and second generation triple annealed highly cross linked polyethylene. Dislocation rate at the short term is none. Results from this series have to be carefully interpreted due to the relatively short follow up but so far results are encouraging. Long term follow up is required to conclude whether there is early or higher rate of failure. It is our intention to follow up this cohort and further publish our results at longer term.

© 2017

1. Introduction

Around 700,000 hip replacements and 80,000 revision hip replacements have been performed since 2003 according to the 2015 Annual Report of the National Joint Registry.¹ With better understanding of material properties and development of manufacturing principles, hip components continue to evolve.

The NJR Annual Report for 2015 shows an increase in¹ hybrid hip replacement. The use of large diameter heads has increased due to^{2,3} favourable evidence in the recent years. Metal on polyethylene articulation accounts for 87.8% of all cemented hip replacements performed, but only 37.6% of uncemented hip replacements and 63.9% of hybrid hip replacements have metal on polyethylene articulation.¹

Though pain relief had been the primary aim of hip replacement for arthritis, stability, better range of motion and longer survival of prostheses are being sought as younger patients with arthritis are being treated and older patients are more active and have better

* Corresponding author at: Department of Orthopaedics, Princess Royal Hospital, Apley Castle, Telford, TF1 6TF, United Kingdom.

E-mail address: rajikumart129@doctors.org.uk (R. Thangaraj).

life expectancy. When boundaries are pushed, new problems are encountered. For instance, not long ago, there was an upsurge towards metal on metal articulation to prevent wear, hailed as a next step in improved articulation. Fast forwarding, new problems in the form of metal debris with subsequent ALVAL reaction and pseudo tumour resulted in less than 1% hip replacements being performed with metal on metal articulation as per NJR 2015.¹

Large diameter heads have higher wear rates due to their larger sliding distances.^{4,5} Success of Charnley's low frictional torque arthroplasty^{4,5} is due to the use of smaller 22 mm diameter heads, as the higher frictional torque generated by the larger heads due to increased sliding distance caused higher wear of the polyethylene manufactured in Charnley's era, resulting in early loosening of the components. The disadvantage of the smaller heads has been the dislocation and reduced primary range of motion. With the availability of highly cross linked polyethylene with presumed better wear properties, orthopaedic surgeons around the world have been increasingly using larger heads to achieve better primary arc range of motion and stability and to reduce dislocation rate. Recent studies from the joint registry⁶ has shown no higher rate of failure when large diameter heads were used with highly cross linked polyethylene. Recent evidence^{7–11} have shown satisfactory clinical outcome with low dislocation rate, better range of motion, improved stability with large diameter heads.

Improvement in the manufacturing of polyethylene and the production of highly cross linked polyethylene has aided production of polyethylene with superior wear property, facilitating the use of larger heads. Compared to ultra high molecular weight polyethylene (UHMWPE), the highly cross linked polyethylene (HCLPE)^{12–17} is considered to have better surface wear properties and has a larger surface hardness, making it more scratch resistant and is proven in¹⁸ clinical studies as well. The first generation HCLPE^{19–22} has shown satisfactory clinical performance with good midterm survival and satisfactory survival with² large heads.

The production of HCLPE is now in the second generation with different manufacturers having different principles producing HCLPE with different mechanical properties, although their effect on the tribological properties of the bearing surface is questionable.^{23,24} In vitro studies show similar properties of first and second generation HCLPE in molecular structure and mechanical properties.²⁵ In vitro studies show that HCLPE was better in withstanding higher frictional torque when 40 mm heads were used than conventional UHMWPE. Though HCLPE shows less wear, clinical studies have shown that it is not better than conventional PE when osteolysis or wear-related revision rates are compared.^{21,26}

X3 HCLPE (Stryker, USA) is produced by the second generation manufacturing of sequential processing, whereby the process of irradiation and low heat annealing is done three times. By sequential (triple) annealing or heating and cooling three times to sub melting temperature,²⁷ cross linking is aided and free radicals are abolished to a low level at which they do not cause polyethylene scission, strongly reducing²⁷ the possibility of oxidation.

By improving the wear properties of polyethylene, thinner liners can be used against the large diameter heads. The minimum thickness of triple annealed highly cross linked polyethylene to prevent significant wear is unknown, but evidence of fractures of early generation HCLPE when its thickness was less than 4.8 mm at the rim have been reported.²⁸ On the other hand, the locking mechanism of the thinner first generation HCLPE when used with large diameter heads are considered strong enough, without major concern.²⁹ The safety of the thin liners has been questioned but current³⁰ clinical evidence and³¹ laboratory studies supports satisfactory survival at short term.

With the increase in uncemented acetabular shells for fixation and large femoral heads,^{1,6} the thickness of the liner plays an important role for two reasons. It is extremely difficult to determine the progress of the wear radiologically as the metal shell's shadow overlaps the liner and even if there was a significant wear, an uncemented shell may not show significant evidence of loosening until late. Second, if the polyethylene wears out completely, the Co-Cr metal head will start to articulate with the titanium metal shell, generating large amounts of metal debris potentially causing a metal adverse reaction and pseudo-tumour formation if the polyethylene wear is not detected early.

Evidence for the satisfactory survival of second generation HCLPE in the short to midterm has been published in recent years^{12–15,32–34} but survival of a very thin liner alone has not been reported to our knowledge. Though retrieval studies have shown evidence of oxidation in annealed HCLPE,³⁵ no correlation between oxidation and clinical failure has been found. Although bio-mechanical changes in the HCLPE^{36,37} have been noted, whether these will translate to a clinical early failure is unknown.

With modular hip systems, there is a concern from secondary articulating surfaces between the trunion and femoral heads.^{38–45} The trunion is a Morse taper and the head is wedged on to the trunion. No motion should occur between the surfaces but in reality it is difficult to prevent the micro motion. The micro motion in the smaller heads is not of major concern as the frictional torque generated at the surface is low. As frictional torque is directly proportional to the radius of the head, larger the head, higher is the frictional torque. As the articulation surfaces are metal, the higher frictional torque generates metal debris. Multiple factors like design of the trunion, improper seating of the head, head diameter, metal surface roughness, hardness, soft tissue stiffness, patient factors, time from the index procedure^{46–50} can influence the trunion related metal debris and wear. The major concern is the metal debris from trunion^{38–40,51} causing a metal reaction in the form of ALVAL formation or pseudo tumour formation and early failure of the implants. The diagnosis is difficult though recently it had been noted that⁵² elevated cobalt levels compared to chromium levels is suggestive of trunion wear. Corrosion from the trunion has also been a concern when large diameter head articulating with a small trunion^{38,39,41,49,53} but recent retrieval study has shown the head size⁵⁰ has no effect on corrosion. Apart from higher frictional torque^{38,51,53}, corrosion can also be a cause for metal ion release and metal debris. Head length,^{41,42} size, material^{46–48,54} are thought to influence the fretting and corrosion at the trunion. Though highly cross linked polyethylene has a better wear rate,⁵⁵ recent evidence has shown higher volumetric wear with large diameter heads. Finite element analysis⁴⁴ has shown increase wear potential from trunion with large diameter heads. There has been conflicting evidence questioning the use of large heads with advantages and disadvantages, especially, in relation to trunion wear.^{33,56,57} There have been concerns due to trunion wear for a long time^{40–42,45,53,58,59} with case reports, systemic reviews and retrieval studies being published on failure requiring revision and metal reaction due to debris from trunion articulation. As far as we are aware there are no major clinical studies with large number of patients to suggest the revision rate is higher in an Exeter stem with large diameter head.

The Exeter double taper collarless polished stem is one of the most common implant¹ to be implanted in United Kingdom. The Exeter V40 Taper is a patented design of the Exeter stem and is unique. The material property, design, size, trunion angle are different from other manufacturers and it is unclear whether large diameter 40 mm heads have a negative outcome. Recent studies on the blood metal ion levels from Exeter stem has shown no major concern when used with 36 mm heads.⁶⁰ The thinnest second generation highly cross linked polyethylene (3.8 mm) is implanted

on a 50 or 52 mm trident uncemented acetabular shell (Stryker, USA) and will articulate with a 40 mm heads while the liners in the smaller shells less than 50 mm will only articulate with 36 mm heads and are thicker. The trident uncemented acetabular shell (Stryker, USA) of size 54 mm or more have thicker second generation highly cross linked polyethylene (3.8 mm).

The primary aim of this study is to assess if any early failure is noted when large diameter 40 mm heads are used against second generation triple annealed highly cross linked polyethylene acetabular liners in hybrid hip replacements with Exeter stems and to assess survival at short term. As a secondary aim we also assessed the survival of the thinnest second generation highly cross linked polyethylene (3.8 mm). As far as we are aware, this is the thinnest polyethylene manufactured and we felt that this has to be reported as a subset of our cohorts.

2. Methods

A retrospective case series of patients who had hybrid hip replacements with 40 mm heads on an Exeter stem articulating against second generation triple annealed highly cross linked polyethylene liner on an uncemented hydroxy apatite coated Trident acetabular shell was performed. Ethical approval was obtained (IRAS id no. 198853, 198872) for the project. All patients had hybrid hip replacements for primary osteoarthritis.

All patients treated at our unit under a single surgeon (RDP) were identified from hospital records and the National Joint Registry for England, Wales, Northern Ireland and the Isle of Man (NJR). Survival of the implants was confirmed from the NJR as any revision of the component were reported and recorded in this registry. Individual records, electronic patient records and radiographs of all included cases were reviewed. Radiographs were reviewed to assess for any significant progressive loosening of components. Complications in term of leg length discrepancy, infection, dislocation, neurological damage and any other complication were noted. We searched for cases of failure due to any reason in both hospital records and the NJR data base with revision for any cause being considered the end point. Hospital records were reviewed to assess if any case had developed metal reaction or pseudotumour as this might signify catastrophic wear, with the metal head most likely articulating with the titanium shell, producing large amounts of metal debris. Implant survival was determined using the Kaplan-Meier method and Peto estimates of the 95% confidence intervals, which take account of the effective sample size. All statistical analyses were performed using R vs 3.0.2, using the “survival” package.

3. Results

324 hybrid hip replacements with 40 mm large diameter metal Co-Cr alloy heads on a cemented Exeter femoral stem articulating with second generation highly cross linked polyethylene on an uncemented trident acetabular shell had been performed through posterior approach for primary hip osteoarthritis between 2006 and 2014. Of the 324 patients, 165 were female and 159 were male patients. Age range was from 42 to 88 with an average of 70.5 years (± 0.9 years at 95% CI) at the time of procedure [Median 71, SD 8.3 years].

154 of the 324 hip replacements had the thinnest second generation highly cross linked polyethylene (3.8 mm). There were 128 female and 26 male patients. There were more female patients in this subset due to relatively smaller acetabular size in females. The average age at the time of surgery was 71.8 years (7.3SD, range 42–88 years).

At the time of the data collection for the study, none of the patients had dislocation. None of the implants had been revised for

aseptic loosening or significant wear or due to trunion related wear. None of the hip replacements had been revised for pseudo tumour formation or ALVAL reaction. Examination of radiographs found no evidence of noticeable osteolysis. 34 patients had died due to non orthopaedic causes of cardiac or disseminated malignancy.

Revision for any cause was considered as end point. 2 patients had revision of the components. 1 patient had deep infection requiring 2 stage revisions. This patient had large diameter 40 mm head with thinnest second generation highly cross linked polyethylene. One patient had a fall and sustained pelvic fracture involving the columns and the acetabular shell lost the fixation and had to be revised following the column fixations and head was changed to 36 mm. An analysis of the NJR data confirmed that this was indeed the only two cases that had revision in this series as of end of 2015.

Other complications noted in our series were as below but none of them had revision of the components. 1 patient had foot drop which recovered. 1 patient had sciatic nerve damage and had nerve repair and later foot procedure for the foot drop under the foot and ankle team. One patient had CVA in the post operative period. 2 had superficial infection treated with oral antibiotics but did not require revision. 6 had limb length discrepancy requiring heel rises. 19 had back pain due to spinal degenerative causes. 7 developed trochanteric pain due to trochanteric bursitis. One settled with steroid injection but others did not require any treatment and symptoms settled with conservative management.

The patient (58/F) who had a steroid injection had no further symptoms. Comparison of immediate postoperative radiograph (Fig. 3) and 7-year follow up radiograph (Fig. 4) showed no evidence of osteolysis or loosening. A further example of radiographic follow up is a 70 year old female with a follow up of over 7 years, which again show no signs of osteolysis when comparing between immediate postoperative (Fig. 5) and latest follow up (Fig. 6).

Probability of survival (%)

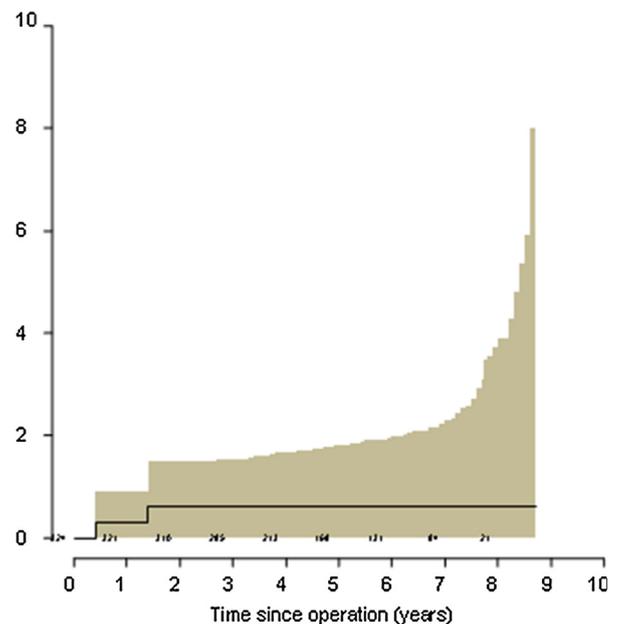


Fig. 1. Kaplan-Meier Survival curve of 40 mm Heads on cemented Exeter stem articulating with all HCLPE X3 on uncemented trident acetabular shell showing 99.4% at 7.8 years but a widened confidence interval towards the right side – grey shaded area shows confidence interval.

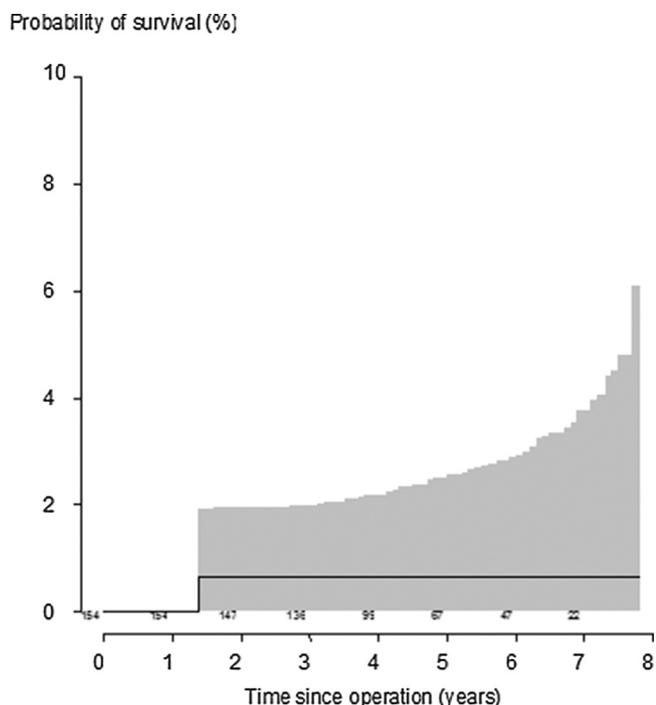


Fig. 2. Kaplan–Meier Survival curve of thinnest (3.8 mm) HCLPE X3 on uncemented trident acetabular shell articulating with 40 mm Heads on cemented Exeter stem showing 99.3% at 8 years but a widened confidence interval towards the right side – grey shaded area shows confidence interval.

Kaplan–Meier survival analysis of the 324 hip replacements with 40 mm large diameter metal Co–Cr alloy heads on a cemented Exeter femoral stem articulating with second generation highly cross linked polyethylene on an uncemented trident acetabular

shell showed the 5-year survival probability of the implant was 99.4% (95% CI 98 to 100%), corresponding to a failure probability of 0.6% (95% CI 0.0 to 2%; Fig. 1). At latest follow up (7.8 year) the probability of survival was the same but with a wider 95% confidence interval (88.8 to 100%) (Fig. 1).

Kaplan–Meier survival analysis of 154 hip replacements with thinnest second generation highly cross linked polyethylene (3.8 mm) showed the 5-year survival probability of the implant was 99.3% (95% CI 97.1 to 100%), corresponding to a failure probability of 0.7% (95% CI 0.0 to 2.9%; Fig. 2).

4. Discussion

The study had shown satisfactory survival of 40 mm large diameter metal Co–Cr alloy heads on a cemented Exeter femoral stem articulating with second generation triple annealed highly cross linked polyethylene [X3 HCLPE] on an uncemented trident acetabular shell for primary hip osteoarthritis at short term. The subset of hip replacements with the thinnest (3.8 mm) HCLPE liner at short to midterm also shows satisfactory survival at short term.

Concerns of wear due to increased frictional torque generated by the large sliding distances of the large diameter heads at primary and secondary articulation surfaces had restricted the use of large diameter heads and our series had shown satisfactory survival at short term. Though trunion related wear has been considered a problem to deal with the modern modular femoral stems, the V40 taper of the Exeter femoral stem has shown satisfactory resilience against trunion wear in spite of higher frictional torque produced by the large diameter heads as none of hip replacements in this series had been revised for trunion related problems at short term.

Despite testing in its thinnest form against the largest available head, producing the largest sliding distance with a maximum frictional torque, so far the survival of second generation triple



Fig. 3. 58y/F had right THR for Primary OA. Patient had trochanteric pain settled following steroid injection.



Fig. 4. 6 year postoperative radiograph – patient has no symptoms with hip with satisfactory outcome. Components show no significant loosening.

annealed highly cross linked polyethylene [X3 HCLPE] is satisfactory. We had no dislocation in our series. This combination of a low dislocation rate and good survival at short term suggests this liner

might be an option for use of 40 mm heads in elderly patients as an alternative to dual mobility or constrained liner. No case has been revised so far for aseptic loosening, nor have we seen noticeable

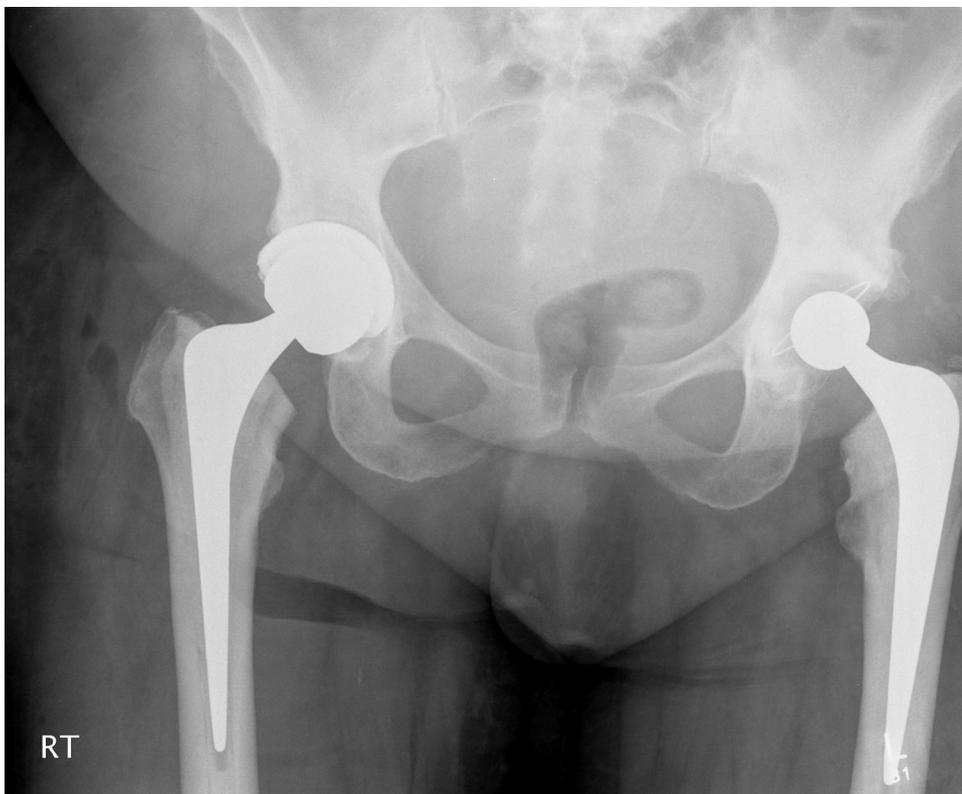


Fig. 5. 70Y/F had right THR for primary OA. Postoperative radiograph after the surgery. Patient had no pain and satisfied. Patient had one of the longest follow up in our series. Patient had left THR with 28 mm head in the past.



Fig. 6. 7 year postoperative radiograph – patient has no symptoms with hip and satisfactory outcome. Minor asymptomatic heterotopic ossification noted but components are not loose.

osteolysis suggesting impending failure. The only revision done was for infection in a patient in two stages and for periprosthetic fracture.

Our results looked at the survival of this polyethylene at its currently thinnest level which reflects the clinical performance. Its low failure rates in this form suggest that the material will also perform well when used with thicker liners for larger uncemented shells. However, it will be difficult to predict if these findings extend to cemented acetabular shells as their fixation is different. It is our intention to follow up this group further and publish the longer-term results to investigate the survival of these thin polyethylene liners.

There is significant restriction in the study. The study is a retrospective case series with short term results. At the study time, revision rate has been extremely low but as years progress there might be higher revision rate due to unknown or known factors. The Kaplan Meier survival analysis in Fig. 1 shows satisfactory survival at 8 years but towards the right side of the curve there is significant widening of the confidence interval.

The study is not without its weaknesses. Firstly, to assess revision rates we relied mainly on the NJR. The time to follow up in the clinic varied because local policy and guidelines had changed during the study period, with patients increasingly followed up at primary care centres for financial reasons. For this reason, the authors relied on the NJR data for the survival of implants. The authors feel that this is justified as all revisions in England, Wales, Northern Ireland and the Isle of Man, are meticulously reported, and our patients have not moved outside the NJR area. Obviously it is not clear whether the high survival found in this study holds in the long run. Other limitation is the lack of patient related outcome scores.

Unfortunately, we were not able to determine the wear rate as this is difficult to achieve with an uncemented shell in situ.

However, we did not find noticeable osteolysis around the femoral or acetabular bone interface when reviewing the radiographs at the latest follow up. A final weakness is that we only studied patients with primary osteoarthritis. It is unclear if the results are reproducible if the above components are used for secondary osteoarthritis.

As hip prostheses continue to develop with advances in material science, bearing technology and manufacturing processes, vigorous monitoring regarding the performance of the newer technologies with publication of results is needed. At the moment, the hybrid hip replacements with large diameter 40 mm heads on an Exeter stem articulating with second generation sequentially processed HCLPE has shown satisfactory survival but longer term follow up is required. It is our intention to further follow this cohort of patients to study the longer term clinical results and safety of the large 40 mm Co-Cr metal heads and second generation sequentially annealed highly cross linked polyethylene and publish our results.

Conflict of interest

The above study has not been published before in any journals in any other format. The manuscript has been read and approved by all authors. All authors believe that the manuscript represents honest work.

Each author certifies that he or she has no commercial associations (eg, consultancies, stock ownership, equity interest, patent/licensing arrangements, etc) that might pose a conflict of interest in connection with the submitted article.

There is no conflict of interest among the authors during the study or in preparing the manuscript nor did the authors receive any funding towards the publication of the case report.

References

- National Joint Registry. 12th Annual Report. 12th Annu Rep. 2015. :81–88 12 (December 2014).
- Sachde B, Maru ND. Mid-term results of large diameter heads on cross-linked polyethylene liners in total hip replacement. *J Clin Orthop Trauma*. 2012 Dec;3(2):94–97.
- Geller JA, Malchau H, Bragdon C, Greene M, Harris WH, Freiberg AA. Large diameter femoral heads on highly cross-linked polyethylene: minimum 3-year results. *Clin Orthop Relat Res*. 2006;447(June):53–59.
- Wroblewski BM, Siney PD, Fleming PA. Charnley low-friction arthroplasty: survival patterns to 38 years. *J Bone Joint Surg Br*. 2007;89(August):1015–1018.
- Wroblewski BM, Siney PD, Fleming PA. The principle of low frictional torque in the Charnley total hip replacement. *J Bone Joint Surg Br*. 2009;91(July):855–858.
- Allepez A, Havelin L, Barber T, et al. Effect of femoral head size on metal-on-HCPE hip arthroplasty outcome in a combined analysis of six national and regional registries. *J Bone Joint Surg Am*. 2014;96(December (Suppl. 1)):12–18.
- Banerjee S, Pivec R, Issa K, Kapadia BH, Khanuja HS, Mont MA. Large-diameter femoral heads in total hip arthroplasty: an evidence-based review. *Am J Orthop (Belle Mead NJ)*. 2014;43(November (11)):506–512.
- Garbuz DS, Masri BA, Duncan CP, et al. The Frank Stinchfield Award: dislocation in revision THA: do large heads (36 and 40 mm) result in reduced dislocation rates in a randomized clinical trial? *Clin Orthop Relat Res*. 2012;470(February (2)):351–356.
- Peters CL, McPherson E, Jackson JD, Erickson JA. Reduction in early dislocation rate with large-diameter femoral heads in primary total hip arthroplasty. *J Arthroplasty*. 2007;22(September (6 Suppl. 2)):140–144.
- Plate JF, Seyler TM, Stroh DA, Issa K, Akbar M, Mont MA. Risk of dislocation using large- vs. small-diameter femoral heads in total hip arthroplasty. *BMC Res Notes*. 2012;5(October):553.
- Van Sikes C, Lai LP, Schreiber M, Mont MA, Jinnah RH, Seyler TM. Instability after total hip arthroplasty: treatment with large femoral heads vs constrained liners. *J Arthroplasty*. 2008;23(October (Suppl. 7)):59–63.
- Callary SA, Field JR, Campbell DG. Low wear of a second-generation highly crosslinked polyethylene liner: a 5-year radiostereometric analysis study. *Clin Orthop Relat Res*. 2013;471(November (11)):3596–3600.
- Callary SA, Solomon LB, Holubowycz OT, Campbell DG, Munn Z, Howie DW. Wear of highly crosslinked polyethylene acetabular components. *Acta Orthop*. 2015;86(April (2)):159–168.
- Epinette J-A, Jolles-Haeberli BM. Comparative results from a national joint registry hip data set of a new cross-linked annealed polyethylene vs both conventional polyethylene and ceramic bearings. *J Arthroplasty*. 2016;31(July (7)):1483–1491.
- Gascoyne TC, Petrak MJ, Turgeon TR, Bohm ER. Wear of a sequentially annealed polyethylene acetabular liner. *Acta Orthop*. 2014;85(September (5)):470–473.
- Glyn-Jones S, Thomas GER, Garfield-Roberts P, et al. The John Charnley Award: highly crosslinked polyethylene in total hip arthroplasty decreases long-term wear: a double-blind randomized trial. *Clin Orthop Relat Res*. 2015;473(February (2)):432–438.
- Pang H-N, Naudie DDR, McCalden RW, MacDonald SJ, Teeter MG. Highly crosslinked polyethylene improves wear but not surface damage in retrieved acetabular liners. *Clin Orthop Relat Res*. 2015;473(February (2)):463–468.
- Digas G, Karrholm J, Thanner J, Malchau H, Herberts P. The Otto Aufranc Award. Highly cross-linked polyethylene in total hip arthroplasty: randomized evaluation of penetration rate in cemented and uncemented sockets using radiostereometric analysis. *Clin Orthop Relat Res*. 2004;(December (429)):6–16.
- Lachiewicz PF, Soileau ES, Martell JM. Wear and osteolysis of highly crosslinked polyethylene at 10 to 14 years: the effect of femoral head size. *Clin Orthop Relat Res*. 2016;474(February (2)):365–371.
- Ranawat CS, Ranawat AS, Ramteke AA, Nawabi D, Meftah M. Long-term results of a first-generation annealed highly cross-linked polyethylene in young, active patients. *Orthopedics*. 2016;39(2):e225–9.
- Snir N, Kaye ID, Klifto CS, et al. 10-year follow-up wear analysis of first-generation highly crosslinked polyethylene in primary total hip arthroplasty. *J Arthroplasty*. 2014;29(March (3)):630–633.
- Bragdon CR, Doerner M, Martell J, Jarrett B, Palm H, Malchau H. The 2012 John Charnley Award: clinical multicenter studies of the wear performance of highly crosslinked remelted polyethylene in THA. *Clin Orthop Relat Res*. 2013;471(February (2)):393–402.
- Vrbka M, Necas D, Bartosik J, et al. Determination of a friction coefficient for THA bearing couples. *Acta Chir Orthop Traumatol Cech*. 2015;82(5):341–347.
- Slouf M, Kotek J, Baldrian J, et al. Comparison of one-step and sequentially irradiated ultrahigh-molecular-weight polyethylene for total joint replacements. *J Biomed Mater Res B Appl Biomater*. 2013;101(April (3)):414–422.
- Burroughs BR, Muratoglu OK, Bragdon CR, et al. In vitro comparison of frictional torque and torsional resistance of aged conventional gamma-irradiated polyethylene versus aged highly crosslinked polyethylene articulating against head sizes larger than 32 mm. *Acta Orthop*. 2006;77(October (5)):710–718.
- Johanson P-E, Digas G, Herberts P, Thanner J, Karrholm J. Highly crosslinked polyethylene does not reduce aseptic loosening in cemented THA 10-year findings of a randomized study. *Clin Orthop Relat Res*. 2012;470(November (11)):3083–3093.
- Miller MD, Thompson SR, Hart JA, eds. Review of Orthopaedics; 2012. 388 p.
- Ast MP, John TK, Labbisiere A, Robador N, Della Valle AC. Fractures of a single design of highly cross-linked polyethylene acetabular liners: an analysis of voluntary reports to the United States Food and Drug Administration. *J Arthroplasty*. 2014;29(June (6)):1231–1235.
- Murtha AS, Roy ME, Whiteside LA, Tilden DS, Schmitt KL. Thin-walled cross-linked acetabular liners need not exhibit reduced locking strength. *Orthopedics*. 2015;38(August (8)):e727–32.
- Jauregui JJ, Naziri Q, Pierce TP, et al. Is the use of thin, highly cross-linked polyethylene liners safe in total hip arthroplasty? *Int Orthop*. 2016;40(April (4)):681–686.
- Johnson AJ, Loving L, Herrera L, Delanois RE, Wang A, Mont MA. Short-term wear evaluation of thin acetabular liners on 36-mm femoral heads. *Clin Orthop Relat Res*. 2014;472(February (2)):624–629.
- D'Antonio JA, Capello WN, Mesko JW, Ramakrishnan R. Second-generation annealed highly crosslinked polyethylene has low wear at mean seven year follow-up. *Surg Technol Int*. 2014;25(November):219–226.
- Sayed SA, Mont MA, Costa CR, et al. Early outcomes of sequentially cross-linked thin polyethylene liners with large diameter femoral heads in total hip arthroplasty. *Bull NYU Hosp Jt Dis*. 2011;69(Suppl. 1):S90–4.
- Selvarajah E, Hooper G, Grabowski K, Frampton C, Woodfield TBF, Inglis G. The rates of wear of X3 highly cross-linked polyethylene at five years when coupled with a 36 mm diameter ceramic femoral head in young patients. *Bone Joint J*. 2015;97(November B(11)):1470–1474.
- Kurtz SM, MacDonald DW, Mont MA, Parvizi J, Malkani AL, Hozack W. Retrieval analysis of sequentially annealed highly crosslinked polyethylene used in total hip arthroplasty. *Clin Orthop Relat Res*. 2015;473(March (3)):962–971.
- Dumbleton JH, D'Antonio JA, Manley MT, Capello WN, Wang A. The basis for a second-generation highly cross-linked UHMWPE. *Clin Orthop Relat Res*. 2006;453(December):265–271.
- Jacobs CA, Christensen CP, Greenwald AS, McKellop H. Clinical performance of highly cross-linked polyethylenes in total hip arthroplasty. *J Bone Joint Surg Am*. 2007;89(December (12)):2779–2786.
- Cooper HJ. Diagnosis and treatment of adverse local tissue reactions at the head-neck junction. *J Arthroplasty*. 2016;31(July (7)):1381–1384.
- Cooper HJ, Della Valle CJ. Large diameter femoral heads: is bigger always better? *Bone Joint J*. 2014;96(November B(11 Suppl. A)):23–26.
- Cooper HJ, Della Valle CJ, Berger RA, et al. Corrosion at the head-neck taper as a cause for adverse local tissue reactions after total hip arthroplasty. *J Bone Joint Surg Am*. 2012;94(September (18)):1655–1661.
- Del Balso C, Teeter MG, Tan SC, Howard JL, Lanting BA. Trunnionosis: does head size affect fretting and corrosion in total hip arthroplasty? *J Arthroplasty*. 2016;31(October (10)):2332–2336.
- Del Balso C, Teeter MG, Tan SC, Lanting BA, Howard JL. Taperosis Does head length affect fretting and corrosion in total hip arthroplasty? *Bone Joint J*. 2015;97(July B(7)):911–916.
- Dyrkacz RMR, Brandt J-M, Ojo OA, Turgeon TR, Wyss UP. The influence of head size on corrosion and fretting behaviour at the head-neck interface of artificial hip joints. *J Arthroplasty*. 2013;28(June (6)):1036–1040.
- Elkins JM, Callaghan JJ, Brown TD. Stability and trunnion wear potential in large-diameter metal-on-metal total hips: a finite element analysis. *Clin Orthop Relat Res*. 2014;472(February (2)):529–542.
- Esposito CI, Wright TM, Goodman SB, Berry DJ. What is the trouble with trunnions? *Clin Orthop Relat Res*. 2014;472(December (12)):3652–3658.
- Mistry JB, Chughtai M, Elmallah RK, et al. Trunnionosis in total hip arthroplasty: a review. *J Orthop Traumatol*. 2016;17(March (1)):1–6.
- Munir S, Walter WL, Walsh WR. Variations in the trunnion surface topography between different commercially available hip replacement stems. *J Orthop Res*. 2015;33(January (1)):98–105.
- Nassif NA, Nawabi DH, Stoner K, Elpers M, Wright T, Padgett DE. Taper design affects failure of large-head metal-on-metal total hip replacements. *Clin Orthop Relat Res*. 2014;472(February (2)):564–571.
- Porter DA, Urban RM, Jacobs JJ, Gilbert JL, Rodriguez JA, Cooper HJ. Modern trunnions are more flexible: a mechanical analysis of THA taper designs. *Clin Orthop Relat Res*. 2014;472(February (12)):3963–3970.
- Tan SC, Teeter MG, Del Balso C, Howard JL, Lanting BA. Effect of taper design on trunnionosis in metal on polyethylene total hip arthroplasty. *J Arthroplasty*. 2015;30(July (7)):1269–1272.
- Jacobs JJ, Cooper HJ, Urban RM, Wixson RL, Della Valle CJ. What do we know about taper corrosion in total hip arthroplasty? *J Arthroplasty*. 2014;29(April (4)):668–669.
- Plummer DR, Berger RA, Paprosky WG, Sporer SM, Jacobs JJ, Della Valle CJ. Diagnosis and management of adverse local tissue reactions secondary to corrosion at the head-neck junction in patients with metal on polyethylene bearings. *J Arthroplasty*. 2016;31(January (1)):264–268.
- Carli A, Politis A, Zukor D, Huk O, Antoniou J. Clinically significant corrosion at the head-neck taper interface in total hip arthroplasty: a systematic review and case series. *Hip Int*. 2015;25(1):7–14.
- Lavernia CJ, Iacobelli DA, Villa JM, Jones K, Gonzalez JL, Jones WK. Trunnion-head stresses in THA: are big heads trouble? *J Arthroplasty*. 2015;30(June (6)):1085–1088.
- Lachiewicz PF, Heckman DS, Soileau ES, Mangla J, Martell JM. Femoral head size and wear of highly cross-linked polyethylene at 5 to 8 years. *Clin Orthop Relat Res*. 2009;467(December (12)):3290–3296.
- Rodriguez JA, Rathod PA. Large diameter heads: is bigger always better? *J Bone Joint Surg Br*. 2012;94(November (11 Suppl. A)):52–54.

57. Triantafyllopoulos GK, Elpers ME, Burket JC, Esposito CI, Padgett DE, Wright TM. Otto Aufranc Award: large heads do not increase damage at the head-neck taper of metal-on-polyethylene total hip arthroplasties. *Clin Orthop Relat Res.* 2016;474(February (2)):330–338.
58. Kao Y-YJ, Koch CN, Wright TM, Padgett DE. Flexural rigidity, taper angle, and contact length affect fretting of the femoral stem trunnion in total hip arthroplasty. *J Arthroplasty.* 2016;31(September (Suppl. 9)):254–258.
59. Witt F, Bosker BH, Bishop NE, Ettema HB, CCPM Verheyen, Morlock MM. The relation between titanium taper corrosion and cobalt-chromium bearing wear in large-head metal-on-metal total hip prostheses: a retrieval study. *J Bone Joint Surg Am.* 2014;96(September (18)):e157.
60. Singh R, Manoharan G, Craig P, Collier S, Shaylor P, Sinha A. Blood metal ions after hybrid metal-on-polyethylene Exeter-Trident total hip replacement. *J Orthop Traumatol.* 2016;17(June (2)):149–153.