

BMCRI method for measuring cup anteversion after total hip replacement[☆]



Manjunath K.S.¹, Gopalakrishna K.G.*¹, Hemanth H.P.²

Department of Orthopaedics, Bangalore Medical College and Research Institute, Bangalore, 560002, India

ARTICLE INFO

Article history:

Received 1 November 2016
Received in revised form 2 October 2017
Accepted 11 January 2018
Available online 11 January 2018

Keywords:

Cup ante version
Abduction
Reliability
Validity

ABSTRACT

Study design: Prospective clinical study

Back ground: In total hip replacement the cup placement is critical. Orientation is determined by anteversion and abduction. We have devised a simple geometrical method to calculate anteversion using simple instruments which does not require complicated conversion tables, scientific calculators, trigonometric tables and special x ray equipment.

Objectives: The aim of study is to evaluate the new method in terms of reliability and validity in comparison with other commonly used radiological methods against CT evaluation.

Methodology: In 30 hips of 25 consecutive patients, 13 females and 12 males who underwent primary total hip replacement in our institution, the component version in our method was calculated and compared with CT evaluation of angles. The intra and inter observer reliability were assessed.

Results: Average CT measurement was 23.28 for ante version. We found our method had good correlation with CT calculation with average variability of $\pm 3.9138^{00}$ in planar anteversion and CT methods had excellent intra and inter observer reliability (C.I. = 0.884 to 0.947 & 0.866 to 0.963).

Conclusion: Our method is accurate in comparison with CT (P value > 0.05), which does not need any reference tables, conversion tables, scientific calculators, multiple radiation exposures and not time consuming.

© 2018

1. Introduction

In total hip replacement the cup orientation is critical as inaccurate placement can cause dislocations in long term.^{1,2} The orientation of the cup is described in terms of abduction and anteversion, the three forms of which was defined by D.W MURRAY² in 1934 as anatomical, radiological and surgical anteversion and abduction. Anatomical anteversion is the angle between transverse axes to acetabular axis on transverse plane. Radiological (planar) anteversion is the angle between acetabular axis and coronal plane. Surgical anteversion is angle between

longitudinal axis of pt and acetabular axis projected on sagittal plane.

Planar anteversion is the angle made by the face of the cup to the parasagittal plane of the body in a plane perpendicular to the cup opening plane² (Fig. 1). There are many methods proposed to calculate anteversion from plain AP radiograph.

In the plain radiograph the edge of the cup is projected as ellipse. Using the principles of construction of ellipse many authors have proposed different methods for the calculation of anteversion (Figs. 2–5).

McLAREN³ defined anteversion as quotient of function of maximum and minimum diameters of ellipse and prepared a reference table of quotients for each degree of anteversion (Figs. 7–12).

VISSER and KONINGS⁴ described a complex trigonometric formula using Cartesian coordinates projected on the ellipse (Fig. 14).

AUCKLAND, UTHOFF and BOURNE⁵ described a method using mathematical formula to calculate the minor axis of the ellipse (Fig. 19).

GHELMAN⁶ used fluoroscopy by changing the x ray tube from caudad to cephalad direction until the rays are tangential to cup edges and noting the angle made to the sagittal plane.

[☆] All human and animal studies have been approved by the appropriate ethics committee and have therefore been performed in accordance with the ethical standards laid down in the 1964 Declaration of Helsinki and its later amendments.

* Corresponding author at: Flat no: 106, Ideal apartments, 16th cross, Ideal home township, Rajarajeshwarinagar, Bangalore, 560098, India.

E-mail addresses: kmanjunath215@gmail.com (M. K.S.), gopalkgortho@gmail.com (G. K.G.), drhemanthhp@gmail.com (H. H.P.).

¹ No: 44/10/3, 11th A Main Road, 18th cross, Padmanabhanagar, Bangalore, 560061, India.

² Fort, K.R.Road, Bangalore-560002, India.

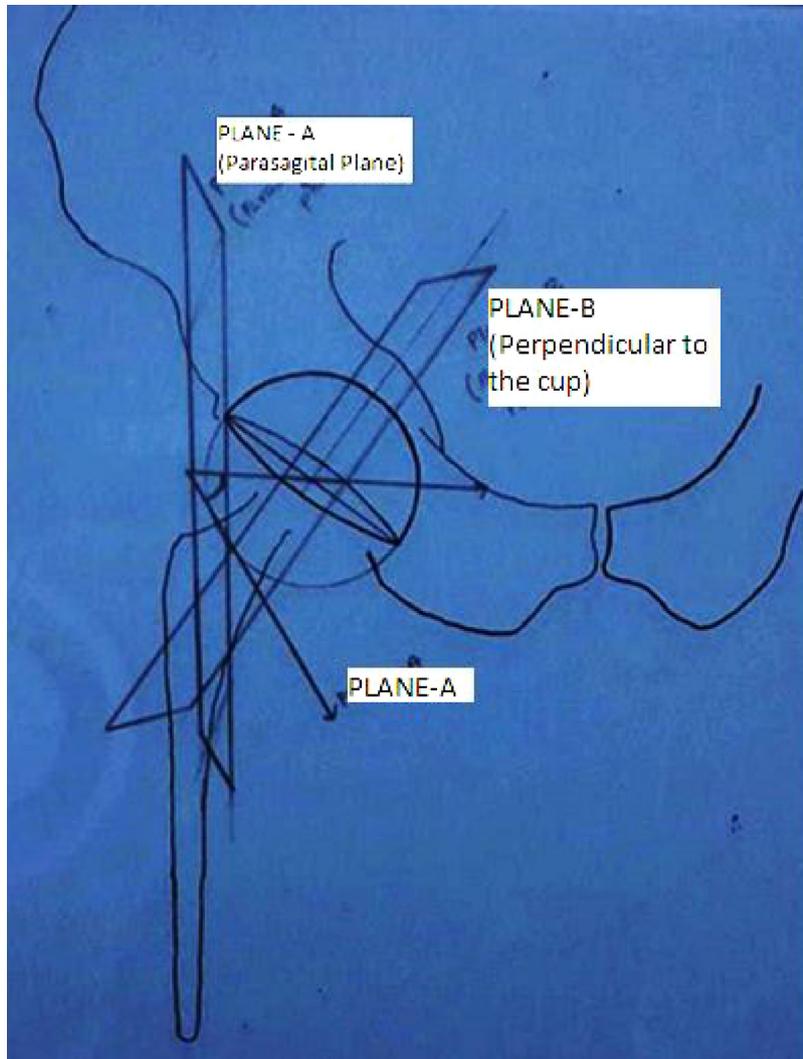


Fig. 1. Planar angle of anteversion.



Fig. 2. AP X-ray of the pelvis in neutral plane.



Two plain AP radiographs, one focusing on pubic symphysis and another focusing on prosthetic head were taken between 3 to 10 days after surgery.

Figs. 3 and 4. Two plain AP radiographs, one focusing on pubic symphysis and another focusing on prosthetic head were taken between 3 to 10 days after surgery. Fig. 3 A-P x-ray centered on Pubic symphysis. Fig. 4 A-P x-ray centered on Prosthetic head.

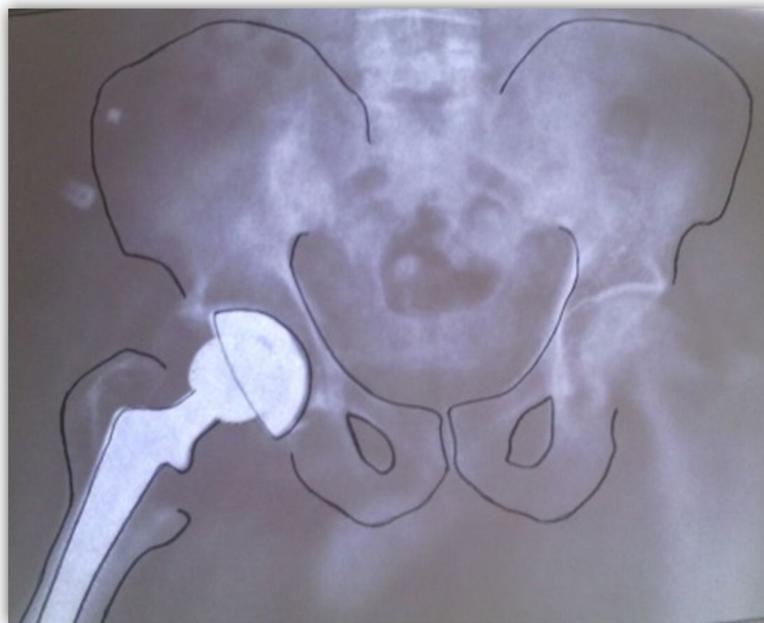


Fig. 5. Superimposed image on trace paper centering on pubic symphysis.

LEWINNEK⁷ used the mathematical formula (Fig. 20) using major and minor axis, sine inverse calculation.

WIDMER⁸ used a formula using minor axis and total length (Fig. 21), sine inverse calculation.

LIAW⁹ used beta angle, sine inverse for the calculation anteversion (Fig. 22)

HASSAN¹⁰ used a complex formula (Fig. 23) involving sine inverse formula

RITHUN used a formula (Fig. 6) using sine inverse formula (Fig. 24)

All these methods use complex trigonometric formula; inter conversion tables and scientific calculator for calculating inverse sine formula. We have devised a method which can directly measure the anteversion angle using simple geometric instruments like divider, compass and protractor.

2. Methodology

We studied 30 hips in 25 patients with 12 males and 13 females in the age-group of 24 to 73 years that were evaluated for

anteversion and abduction by assessing from both plain radiographs and CT measurement.

Indications were avascular necrosis in 20 hips, rheumatoid arthritis in 6 hips, secondary arthritis due to fracture neck of femur in 2 hips; post traumatic in 1 hip and GCT proximal femur in 1 hip.

We excluded patients with fixed pelvic obliquity, revision THR, gross pelvic asymmetry and those contraindicated for radiation exposures.

The x-ray beams were focused perpendicular to body from a distance of 110 cm. The pelvic tilt is corrected by making anterior pelvic plane parallel to the ground. Anterior pelvic plane is formed by three points. The three points are two ASIS and Pubic symphysis which should be on the same level to form the anterior plane and this plane should be parallel to the ground. This is ensured by placing a hard cardboard over these three points and adjust the pelvis tilt to make the anterior plane parallel to the ground

Steps of tracing the cup on the tracing paper.

The edge of cup is imposed on the plain film in the form of hemi ellipse.



Fig. 6. Superimposed image on trace paper centering on prosthetic head.

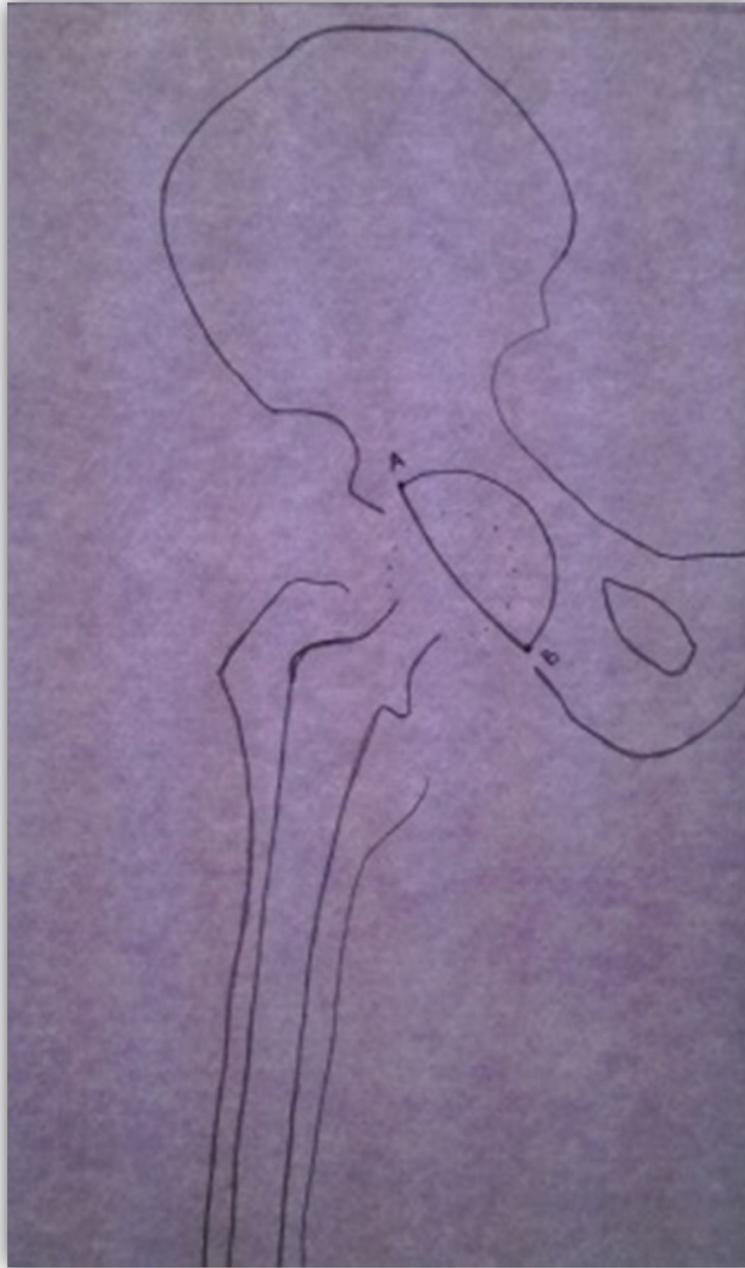


Fig. 7. Tracing the ellipse formed by the mouth of the cup.

The ellipse is completed using pencil/sketch pen after placing the trace paper over the X-ray image.

The photocopies of constructed ellipse were obtained for further geometrical constructions.

All the patients were subjected to CT scan of pelvis within 10 days post operatively. We used 64 channel MDCT systems with high resolution. The protocol was approved by ethical committee and informed written consent was taken from all patients.

3. Radiological method of calculation of anteversion

3.1. Task 1: to ensure the cup is anteverted and not retroverted

The AP radiographs obtained by focusing on pubic symphysis and prosthetic head were taken and ellipse was completed. The size of the ellipse was compared. If the size increases from pubic symphysis focused to prosthetic head focused means it is in anteversion and retroversion if it decreases.

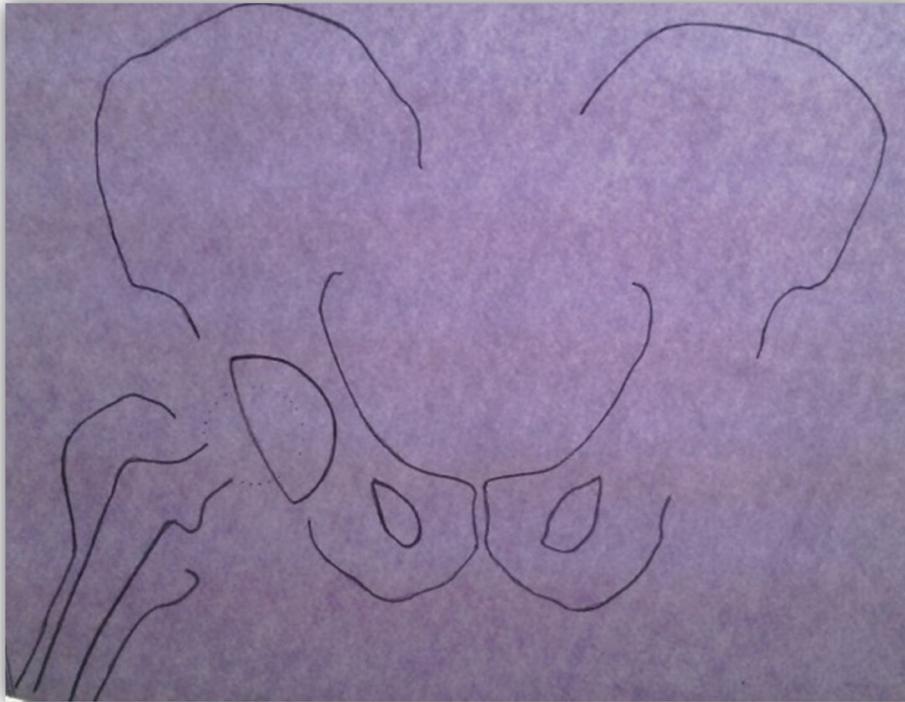


Fig. 8. Tracing the cup dome.

3.2. TASK 2: To determine anteversion by new geometrical method. (Our method . . . hence forth called “BMCRI method”)

FIRST STEP: The photocopy of AP pelvis x ray with reconstructed ellipse is taken. The inter tuberosity line (L-L') is constructed which represents the transverse plane of the body. (Fig. 13)

SECOND STEP: The imaginary axis of rotation of cup is drawn by connecting the two edges of the ellipse. This represents the 'Major Axis'(A-B) around which the face of cup rotates to produce anteversion.

THIRD STEP: The line connecting the two edges of the cup forms the 'major axis' of ellipse. The exact centre of the line is taken as 'C'. (Fig. 15)

FOURTH STEP: Then the other part of ellipse is drawn. With 'C' as centre, half the diameter (half the Major Axis) is taken as radius and an interpolated circle (in RED) is completed such that it just touches the edges of ellipse. (Fig. 15)

FIFTH STEP: From the centre a perpendicular line is towards the edge of the ellipse to complete 'half of the minor axis'(C-D). (Figs. 16 and 17)

SIXTH STEP: Draw another line E-F parallel to the major axis tangentially just at the edge of the ellipse where it touches the minor axis (C-D). (Fig. 18)

SEVENTH STEP: The line E-F cuts the circle at 'O'. Connect C to O. The angle between the line CO and the major axis (C-B) gives the planar ANTEVERSION ANGLE ($\alpha = \alpha$).

3.3. TASK 3: Assessing the anteversion by other radiological methods namely LEWINNEK, WIDMER, HASSAN, LIAW and RITHEN PRADHAN METHOD

Hard copy of each superimposed image was collected and stored. Three surgeons were involved in the calculation of anteversion

in all five methods for all patients. The detailed methodology of measurement was explained to all 3 surgeons and doubts were clarified.

I **LEWINNEK METHOD**⁸: FORMULA FOR VERSION = ARC sine (D1/D2),

D1: minor axis D2: major axis

II **WIDMER METHOD**⁷: FORMULA FOR VERSION = ARCSine (short axis/total length (TL)) = 48.05 multiplied with (S/TL)-0.3 if $0.2 < S/TL < 0.6$. Where S is short axis, TL is the entire distance of the projected cross section of acetabular component along short axis. This method shows linear correlation in the range of S/TL.

III **HASSAN METHOD**⁹: FORMULA FOR VERSION = $\text{ARCSin} \left\{ \frac{(h/D)}{\sqrt{[m/D - m^2/D^2]}} \right\}$. D is the long axis, m is the distance along D not obscured by head, and h is the length of perpendicular dropped from endpoint of distance m to acetabular rim.

IV **LIAW METHOD**¹⁰: FORMULA FOR VERSION = inverse sine tan (beta), where the angle β is obtained by connecting top point of ellipse to the end of long axis.

V **RITEN PRADAN METHOD**¹¹: FORMULA FOR VERSION = ARC sin (P/0.4D), where P is the length of perpendicular dropped from 1/5th of long axis to acetabular rim and D is the long axis.

VI **MEASUREMENT OF VERSION ON CT SCAN**: We used the axial section of CT containing the largest diameter of the acetabular component. A circle was completed touching the edges of the acetabular component/acetabular rim on both the hips. Centres of both circles were identified and a line A was drawn connecting them. The second Line B was drawn perpendicular to the first line passing through the centre. The third Line C was drawn touching the anterior posterior edges of the cup. Now the anteversion is measured as the angle subtended between line B and C.

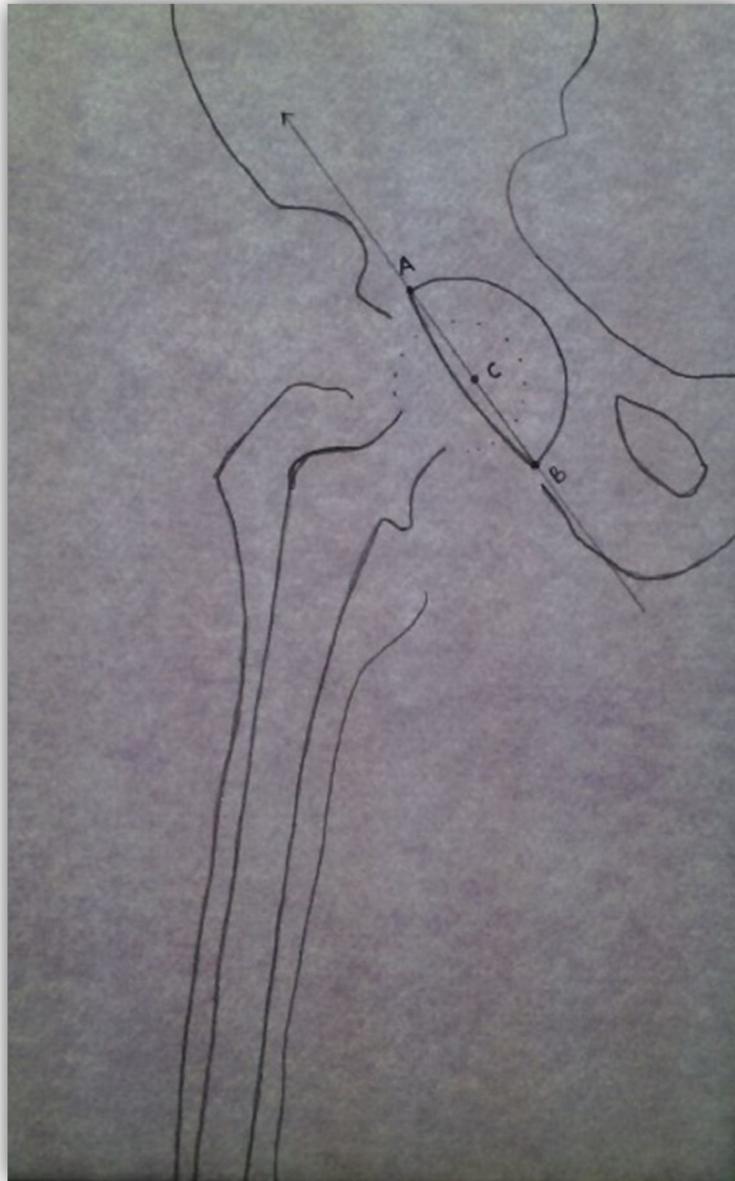


Fig. 9. Major Axis (A-B) drawn from the edge of the ellipse.

4. Results

The intra and inter observer reliability were found to be high. The results for intra observer reliability were calculated by absolute agreement from the readings of the same examiner (Tables 1–3).

5. Measurement of validity

5.1. Validity of different methods

Mean and standard deviation (SD) measurements of each method were compared with the mean of CT measurement using Pearson's correlation coefficient and paired *t*-tests

Discussion:Based on the theory of 'the Geometry of ellipse', the measurement of anteversion of the acetabular cup after THR was done by the methodology on mathematical principles. The opening of the face of the cup is a 'circle' when it is viewed

Table 1
Intra observer reliability in our study.

ICC (INTRACLASS CORRELATION COEFFICIENT)	95% CONFIDENCE INTERVAL
CT – 0.948	0.901 TO 0.964
LEWINNEK – 0.920	0.854 TO 0.960
WIDMER – 0.916	0.859 TO 0.942
LIAW – 0.954	0.884 TO 0.970
HASSAN – 0.904	0.832 TO 0.950
RITEN – 0.920	0.878 TO 0.946
NEW GEOMETRICAL METHOD- 0.903	0.844 to 0.956

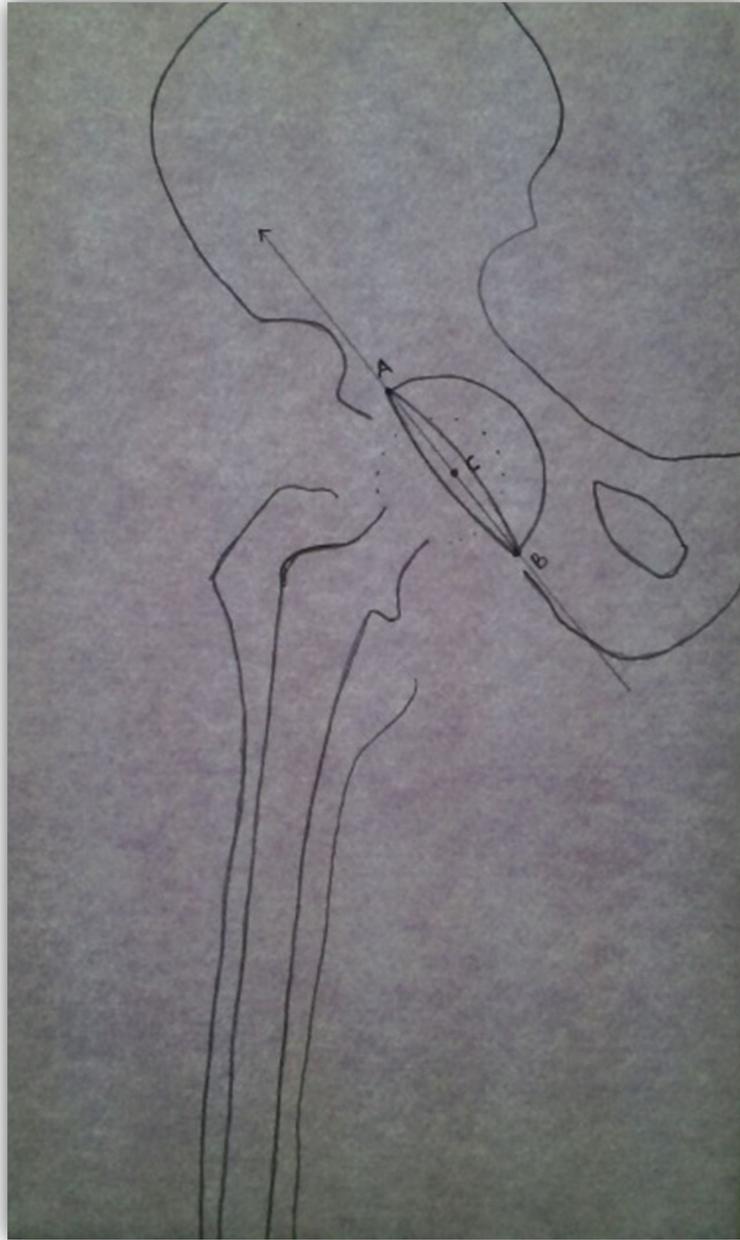


Fig. 10. Completing the ellipse.

perpendicular to its centre. When a circle with AB & CD as its diameters, is rotated around the AB diameter as axis (Major axis), the 'circle face' of the cup start becoming 'ellipse'. On every degree of rotation around the major axis, the circle slowly takes the shape of an ellipse. In simple terms the diameter AB becomes major axis and CD becomes the minor axis of the forming ellipse (Figs. 25–27).

The lines L and L' are tangents to the circle parallel to the AB diameter (Major axis). When the circle is rotated around the axis of AB, the CD diameter (Minor axis) decreases proportionately to

the degree of rotation (C'-D'). The tangents approach closer to each other and to the diameter AB as per the theory of ellipse. These three lines coincide when the face of the cup subtends 0° to the coronal plane (i.e., the line perpendicular to the face of the cup is 0° to coronal plane or anteversion is 0° .) then there is no anteversion in the cup (Fig. 28).

For every degree of rotation around the major axis the tangent line 'L' cuts the original circle at various points 'X' over the circle. As the tangential line moves on the point 'X' over the circle towards the major diameter (major axis), the area of the circle



Fig. 11. The size of the ellipse formed in 'PUBIC SYMPHYSIS CENTERED X-RAY'.

proportionately decreases (forming ellipse) according to the theory of geometry of ellipse (Figs. 29–31).

The axis of the cup dropped to the centre of circle subtends an angle when the circle changes to ellipse. This angle is anteversion (planar).

This three dimensional change (angle) which takes place can be changed to a two dimensional model by connecting center point to x where the tangent cuts original circle. The angle α between line M and AB is the planar anteversion.

6. Assessment of reliability

RELIABILITY is defined as consistency of measurements, calculated by absolute agreement. It is calculated in terms of intra and interobserver reliability.

Table 2
Inter observer reliability.

ICC (INTRACLASS CORRELATION COEFFICIENT)	95% CONFIDENCE INTERVAL
CT – 0.984	0.958 TO 0.990
LEWINNEK – 0.938	0.898 TO 0.966
WIDMER – 0.942	0.902 TO 0.976
LIAW – 0.962	0.914 TO 0.962
HASSAN – 0.908	0.884 TO 0.946
RITEN – 0.914	0.872 TO 0.952
NEW GEOMETRICAL METHOD- 0.953	0.868 TO 0.964

To calculate intra observer reliability one surgeon (JV) measured the ante version in all five methods for all patients two times within a period of four weeks. On the second time the CT and x-ray were distributed to the surgeon (JV) in a random manner.

To calculate the inter observer reliability all 30 hips were evaluated by three surgeons (KSM), (GK), (JV) for all the five methods and the CT method and the results were produced in single statement by absolute agreement. All the measurements were made without any knowledge of clinical information or other surgeons readings.

The ICC and 95% confidence interval were calculated for intra and inter observer reliability. We used two way random effects (intra class correlation model and absolute agreement) to calculate ICC.

An ICC of 1 means perfect reliability and 0 is not at all reliable. ICC values of 0.00 to 0.20 is slight; 0.21 to 0.40 is fair; 0.41 to 0.60 is moderate; 0.61 to 0.80 is substantial; >0.81 is perfect reliability.

7. Measurement of validity

Validity is defined as proximity to reference standard. The validity was calculated by taking mean of anteversion of each method from all the three surgeons and was compared to mean of CT method of measurement of anteversion readings of all three

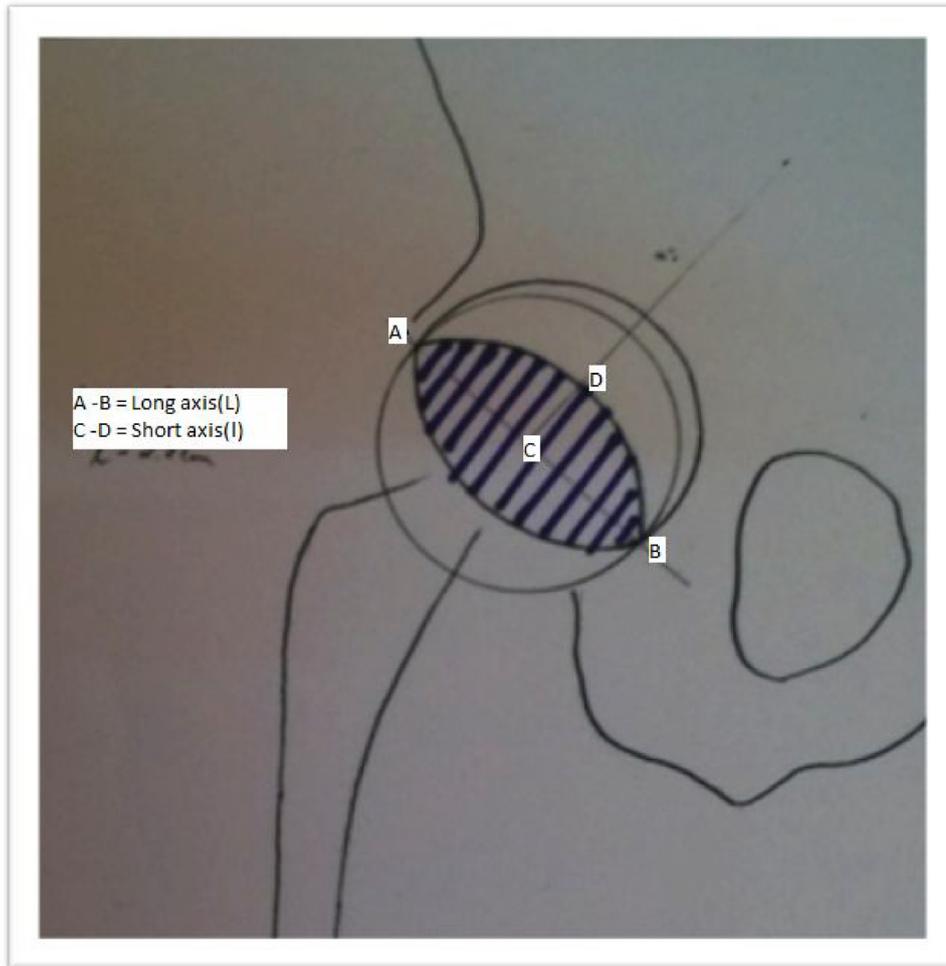


Fig. 12. The increased size of the ellipse (increased short axis) formed on the 'PROSTHETIC HEAD CENTERED X-RAY' indicating cup ANTEVERTED.



Fig. 13. L-L' line = Intertuberosity line.

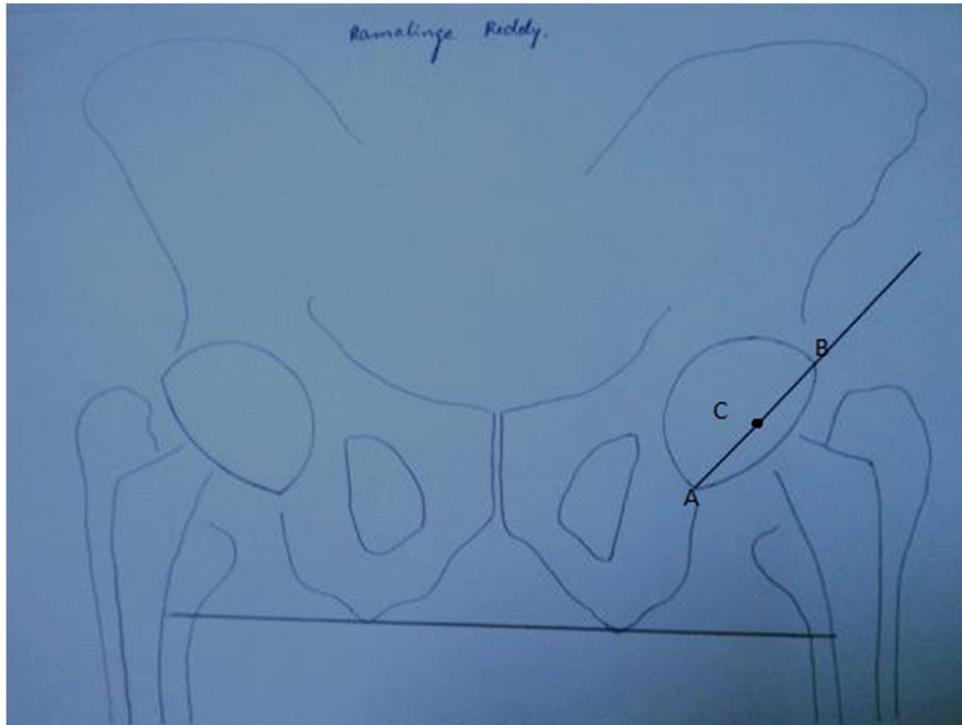


Fig14. A–B = Major Axis.



Fig. 15. C = center of the Major Axis and the ellipse completed by drawing the other half.

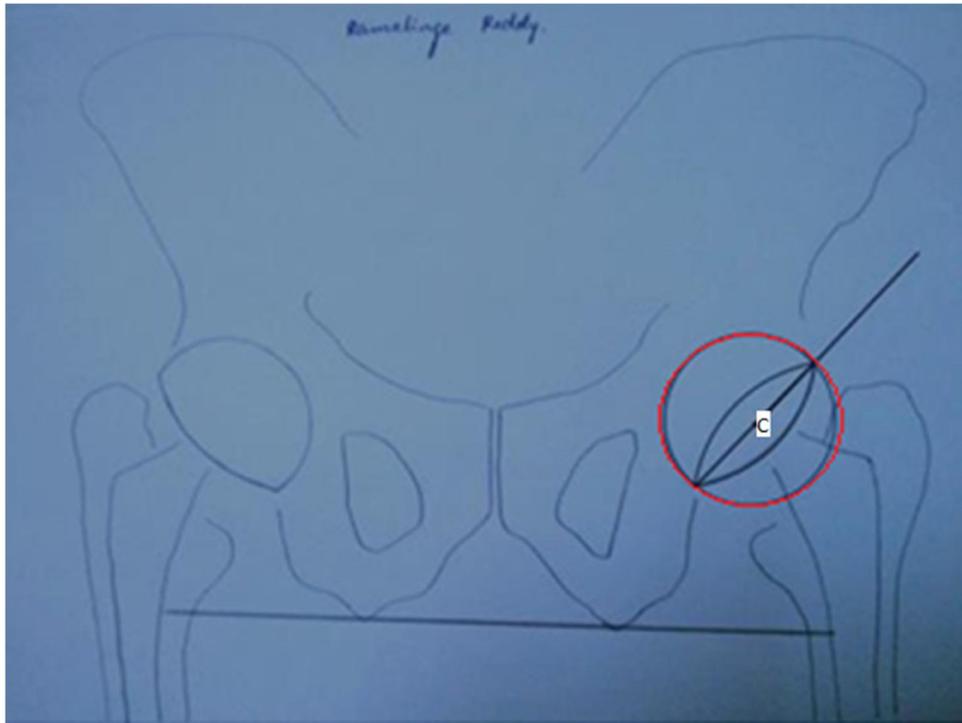


Fig. 16. Interpolated circledrawn from the centre C.

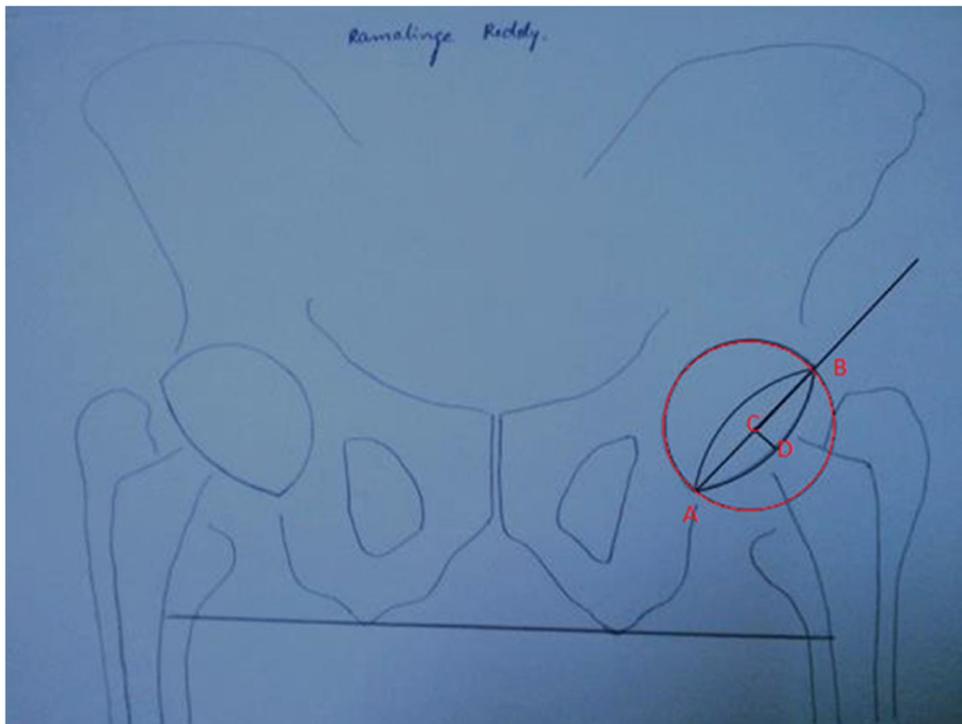


Fig. 17. Half of the Minor axis C-D drawn.

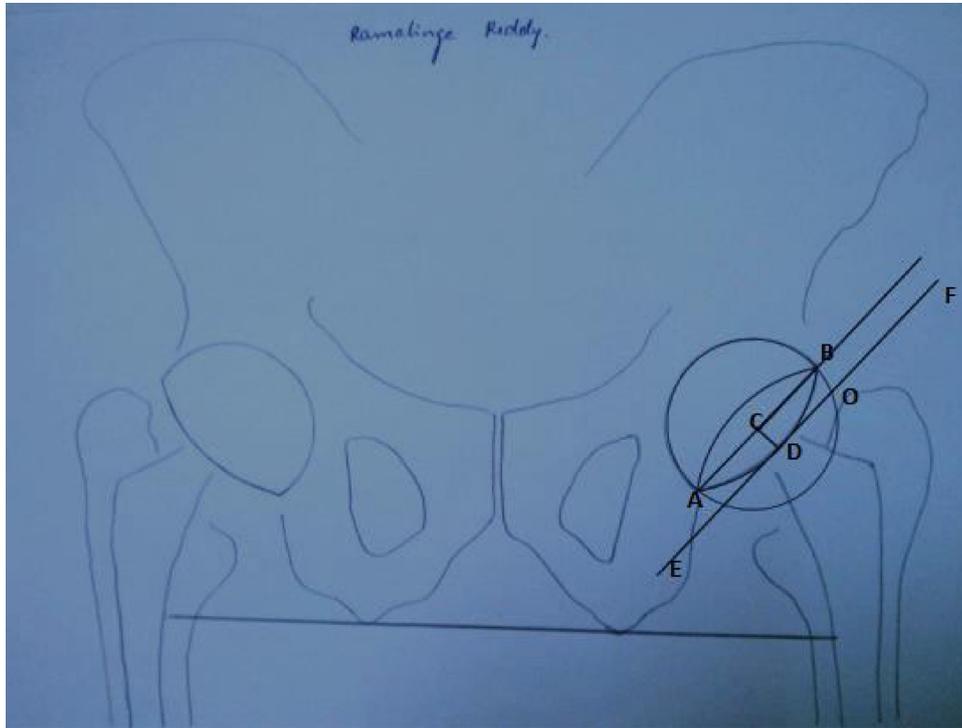


Fig. 18. E-F = Tangential line to ellipse parallel to major axis, O = Point of intersection of EF to the interpolated circle.

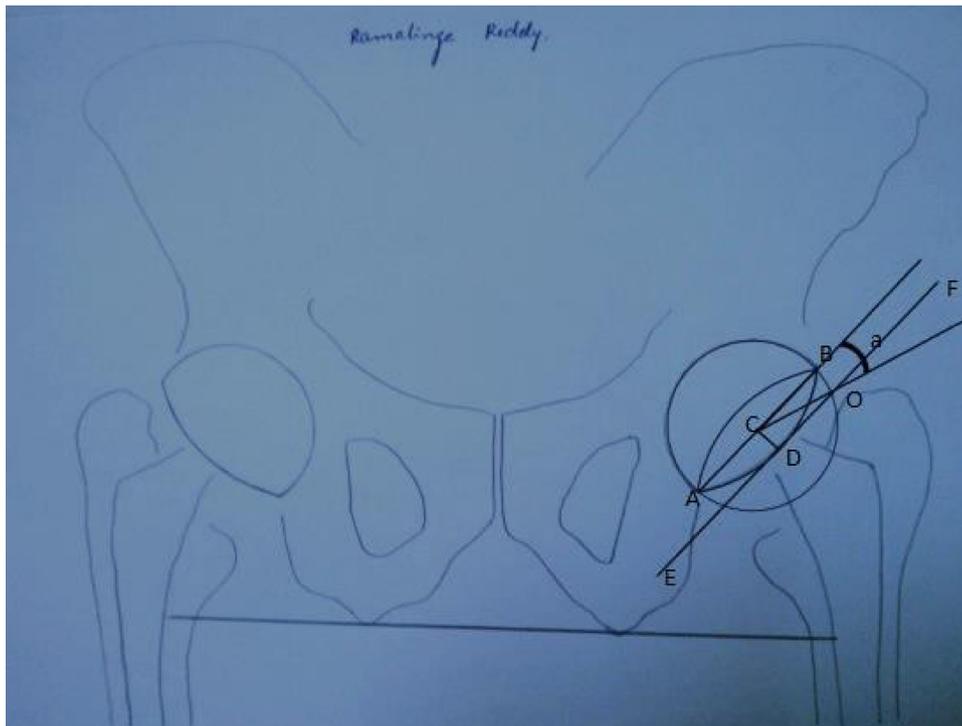


Fig. 19. Anteversion, $a = \alpha$.

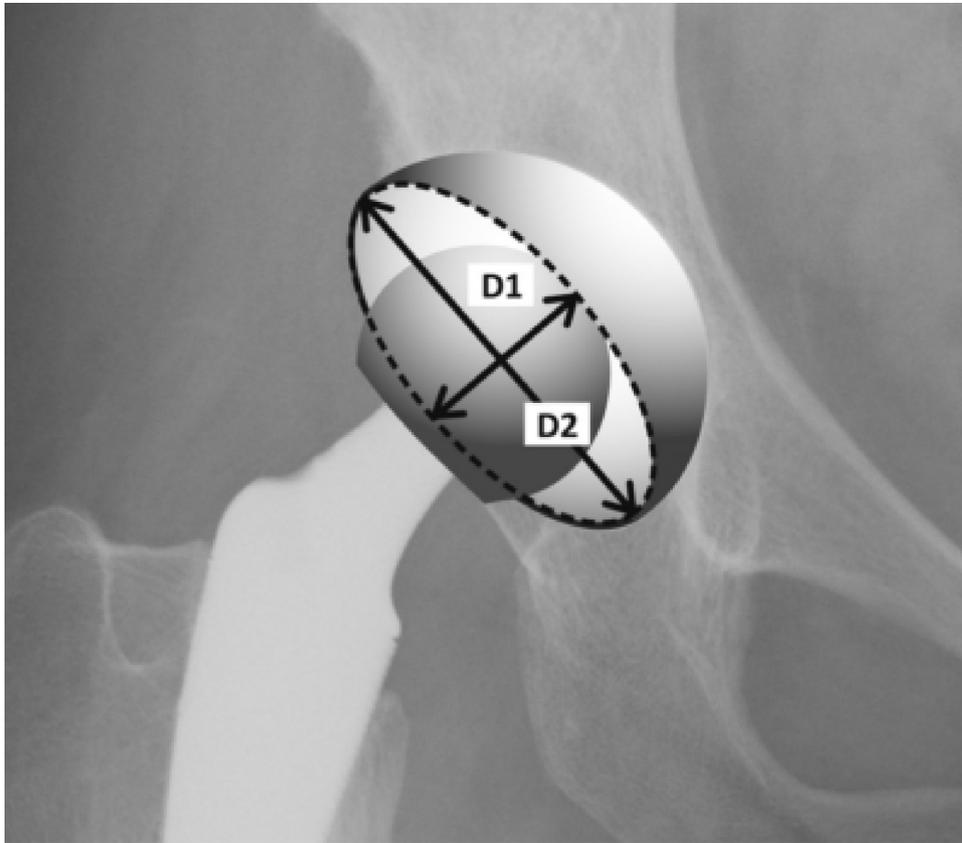


Fig. 20. Lewinnek method.

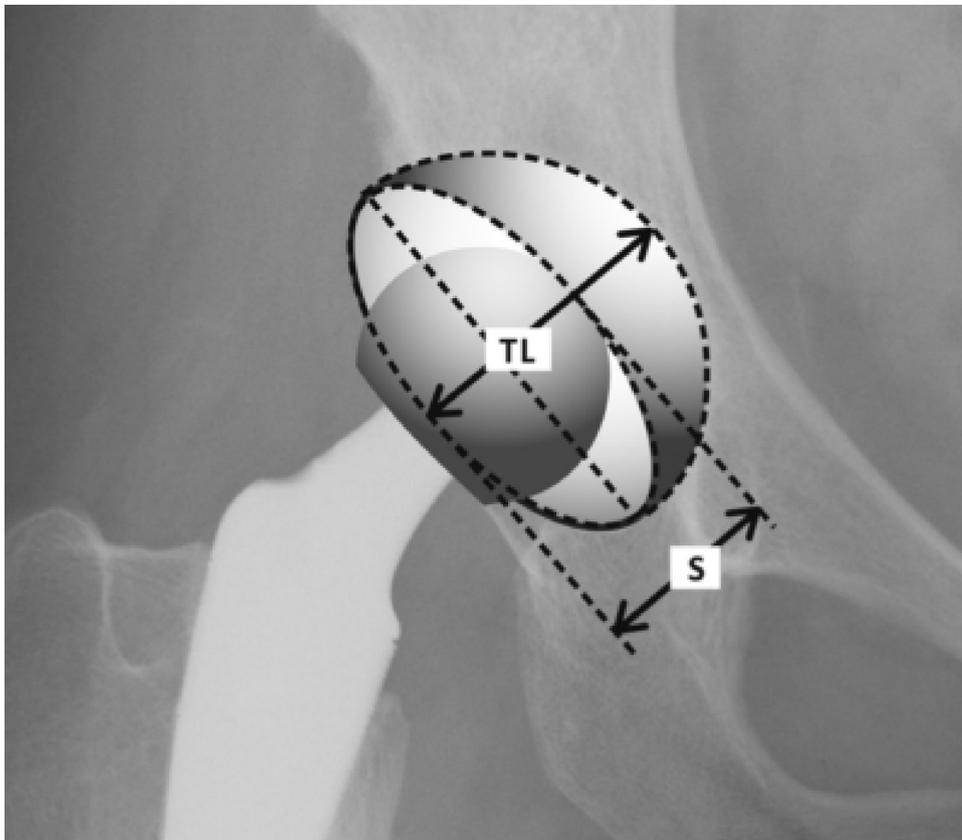


Fig. 21. WIDMER radiological method of calculation of anteversion.

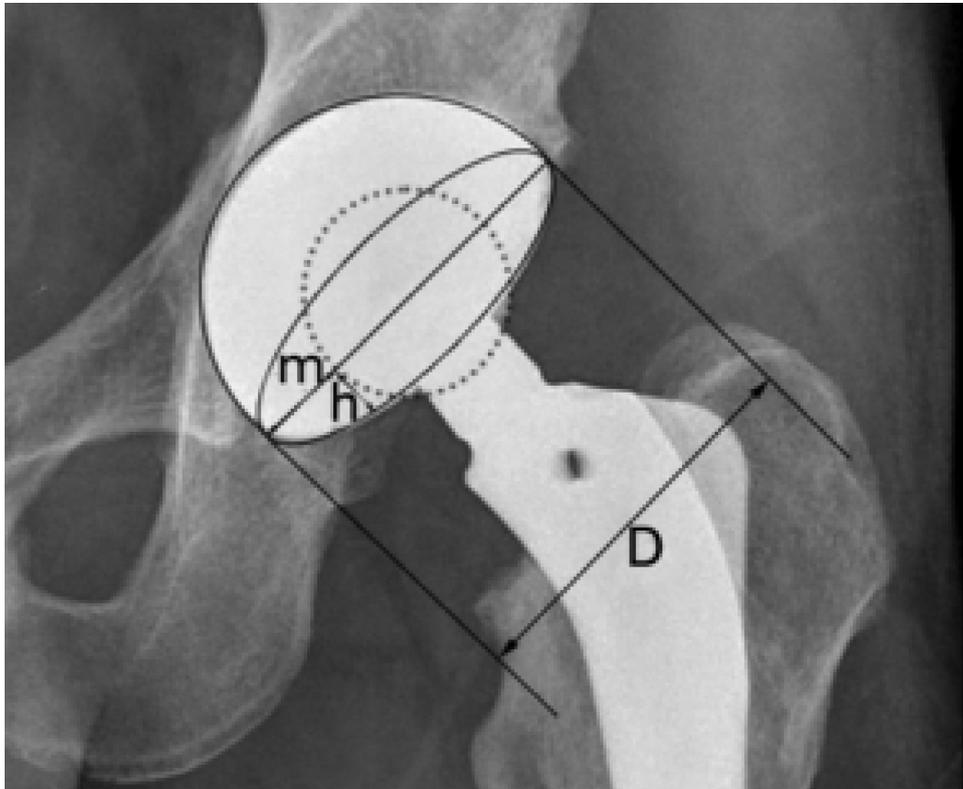


Fig. 22. HASSAN radiological method of calculation of anteversion.

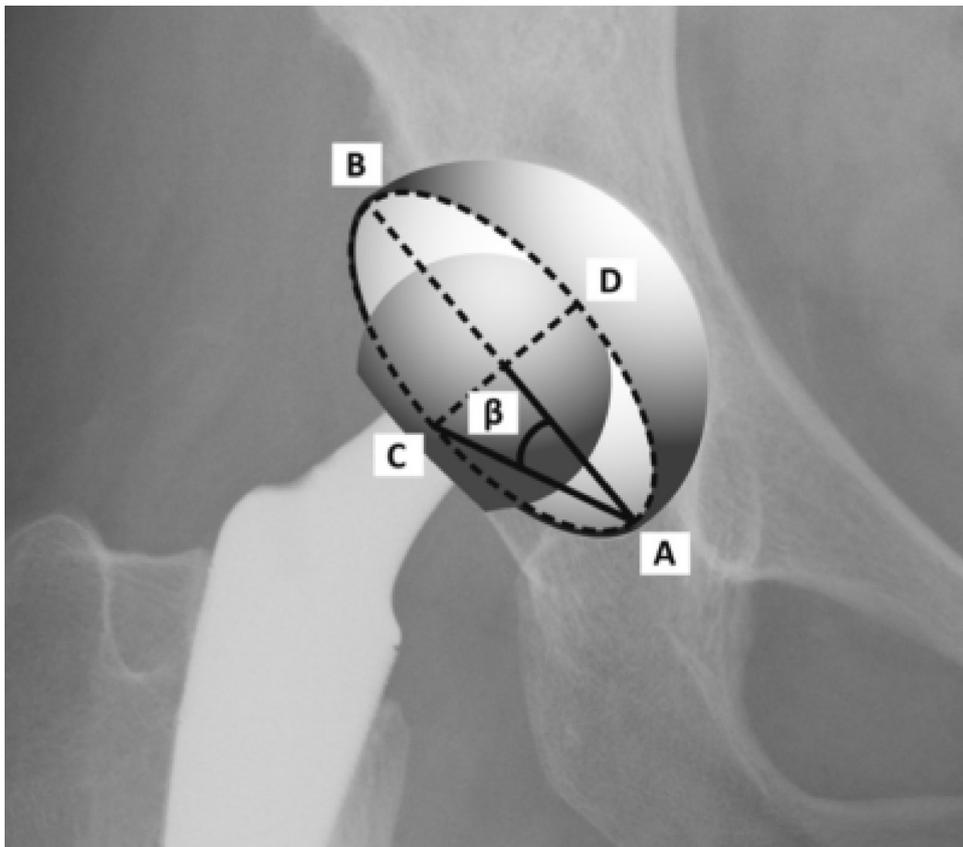


Fig. 23. LIAW radiological method of calculation of anteversion.

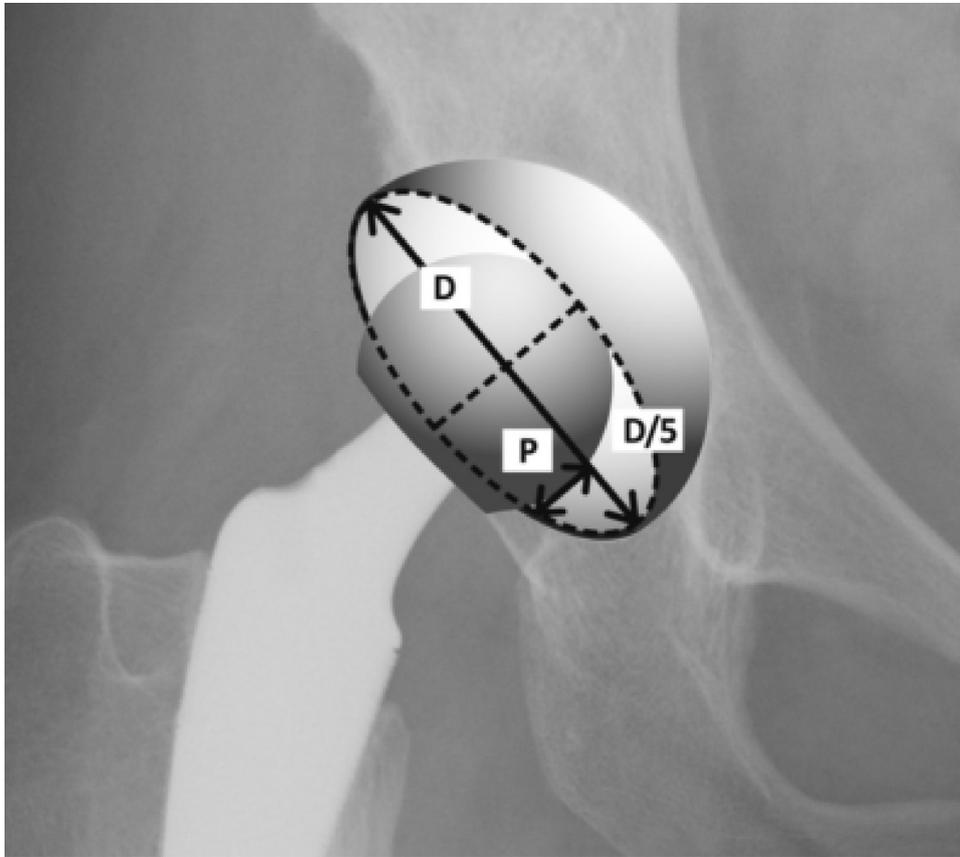


Fig. 24. RITHEN radiological method of calculation of anteversion.

Table 3
Validity of different radiological methods in our study.

Method	Anteversion		As compared to C.T.Scan	
	Mean	S.D.	'p' value As per paired t-tests	Pearson's correlation coefficient
C.T.Scan	23.27	11.93		
Lewinnek	21.65	10.9	0.5899 Not Significant	0.9372
Widmer	31.47	11.7	0.0107 Significant	0.8622
Liaw	21.07	11.04	0.468 Not Significant	0.9193
Hassan	22.4	11.34	0.7757 Not Significant	0.8674
Rithun	22.76	12.12	0.8715 Not Significant	0.8444
NEW GEOMETRICAL METHOD	22.63	10.69	0.8306 Not Significant	0.9318

The radiological measurements of all five methods showed good positive correlations with the CT measurements. The measurements in new method used in this study were similar to the CT measurements (no statistically significant difference)($p > 0.05$, paired t -test).

surgeons. We used paired t -test and PEARSON correlation coefficient with statistical significance set at $p < 0.05$.

PEARSON correlation coefficient is characterised as 'r':- 0.00 to 0.20 = poor; 0.21 to 0.40 = fair; 0.41 to 0.60 = moderate; 0.61 to 0.80 = good and 0.81 to 1.00 is excellent.

7.1. Statistical tools

The information collected regarding all the selected cases were recorded in a Master Chart. Data analysis was done with the help of

computer using Epidemiological Information Package (EPI 2010) developed by Centre for Disease Control, Atlanta.

Range, Frequencies, Percentages, Means, Standard Deviations, Chi Square, 't' value and 'p' values were calculated using this software. Paired 't' test was used to test the significance of difference between quantitative variables. The 'p' value less than 0.05 is taken to denote significant relationship.

Correlation coefficient was calculated using Excel Software. If the value of 'r' between two variables is more than ± 0.5 , then those two variables are taken to be correlated.

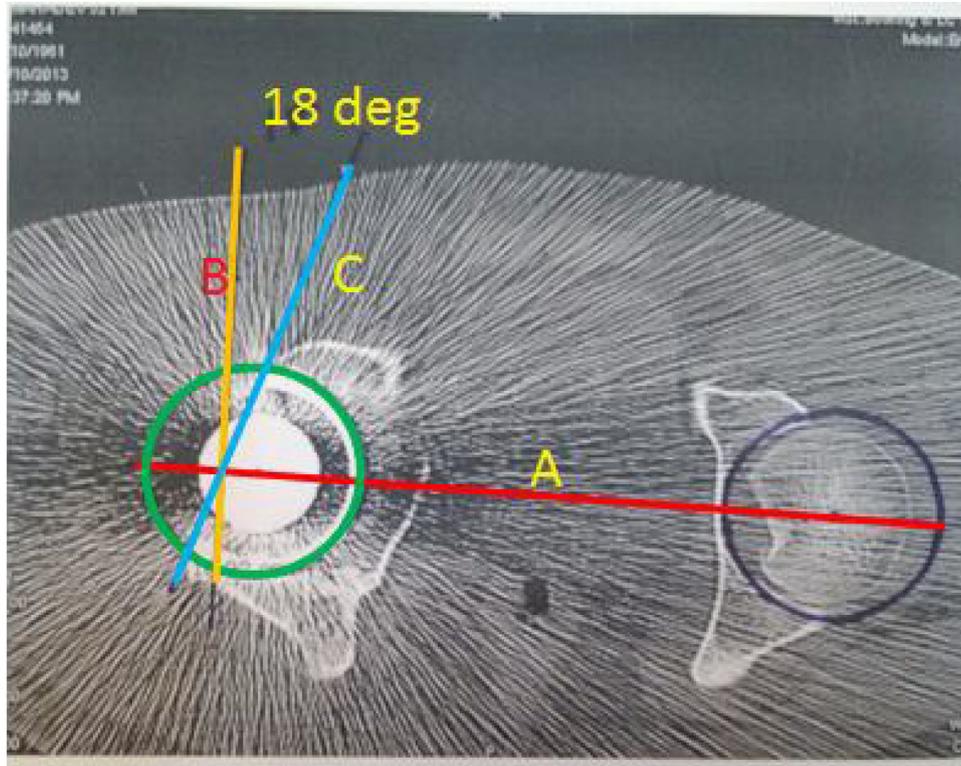


Fig. 25. CT method for measurement of anteversion.

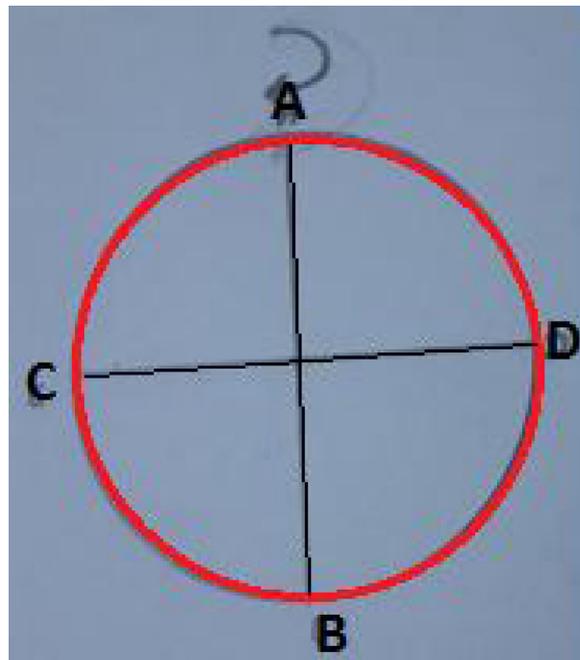


Fig. 26. Full 'circle face' of the cup.

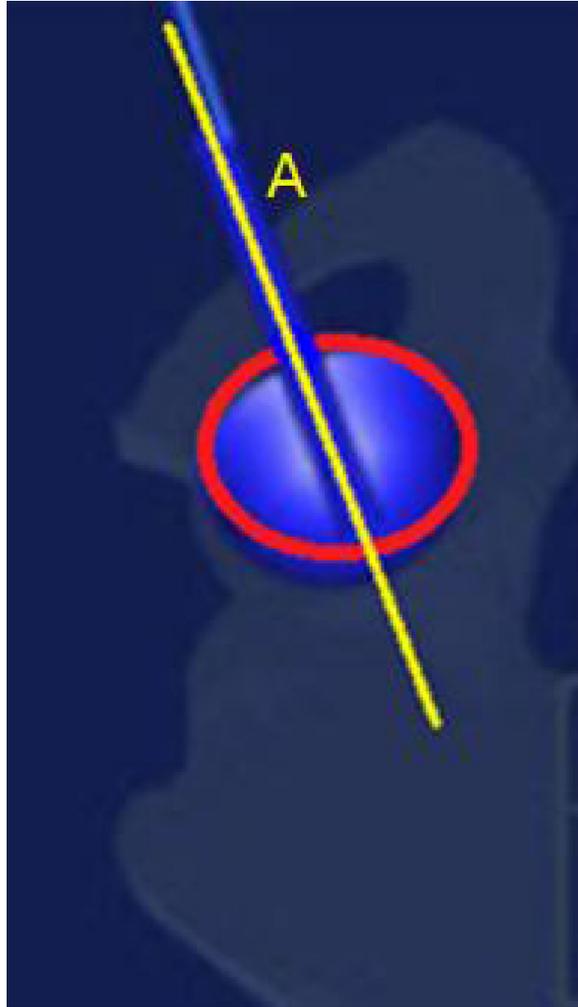


Fig. 29. 'Circle face' (Sagittal face) of cup with its axis 'A' being perpendicular.

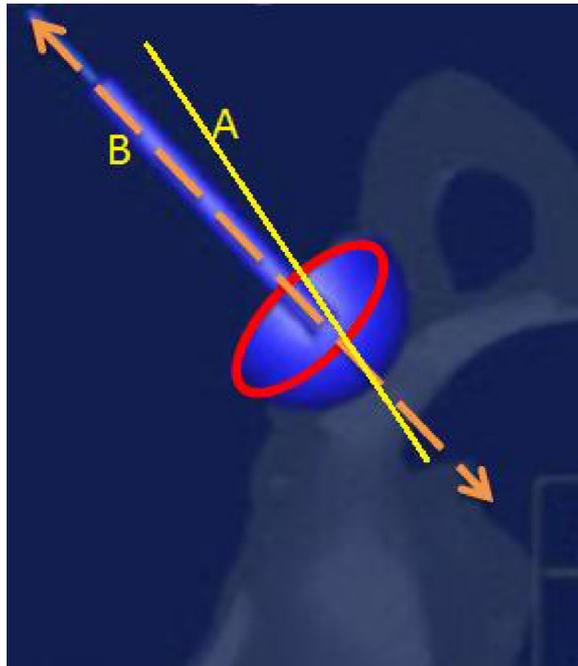


Fig. 30. Coronal face becomes ellipse(anteversion)- axis changes from A to B.

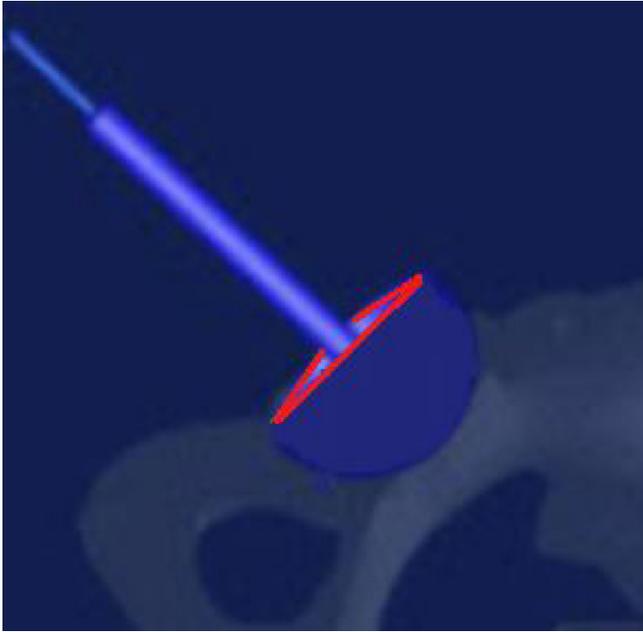


Fig. 31. (0° Anteversion).

8. Conclusion

- Our new method (BMCRI method) is simple, very close to CT scan readings (High validity) and reliable (High reliability).

- In terms of validity our method is better than LEWINNEK method.

Conflict of interest

None.

References

1. Coventry MB, Beckan Baugh RD, Nolan DR, Ilstrup DM. Total hip arthroplasties a study of post-operative course and early complications. *J Bone Joint Surg (Am)*. 1974;56–64.
2. Murray DW. The definition and measurement of acetabular orientation. *J Bone Joint Surg [Br]*. 1993;75-B:228–232.
3. Laren MC. Prosthetic hip angulation. *Radiology*. 1973;107:105–106.
4. Visser JD, Konings JG. A new method for measuring angles after total hip arthroplasty. A study of the acetabular cup and femoral component. *Bone Joint Surg [Br]*. 1981;63-B:556–559.
5. Ackland MK, Bourne WB, Uhthoff HK. Ante-version of the acetabular cup. Measurement of angle after total hip replacement. *J Bone Joint Surg [Br]*. 1986;68-B:409–413.
6. Ghelman B. Radiographic localisation of the acetabular component of a hip prosthesis. *Radiology*. 1979;140:540–542.
7. Widmer KH. A simplified method to determine acetabular cup anteversion from plain radiographs. *J Arthroplasty*. 2004;19:387–390.
8. Lewinnek GE, Lewis JL, Tarr R, Compere CL, Zimmerman JR. Dislocations after total hip-replacement arthroplasties. *J Bone Joint Surg [Am]*. 1978;60-A:217–220.
9. Hassan DM, Johnston GH, Dust WN, Watson LG, Cassidy D. Radiographic calculation of anteversion in acetabular prostheses. *J Arthroplasty*. 1995;10:369–372.
10. Liaw CK, Hou SM, Yang RS, Wu TY, Fuh CS. A new tool for measuring cup orientation in total hip arthroplasties from plain radiographs. *ClinOrthopRelat Res*. 2006;451:134–139.
11. Pradhan R. Planar anteversion of the acetabular cup as determined from plain antero-posterior radiographs. *J Bone Joint Surg [Br]*. 1999;81-B:431–435.