



# The unexplained success of stentplasty vasospasm treatment

## Insights using Mechanistic Mathematical Modeling

P. Bhogal<sup>1</sup> · G. Pederzani<sup>2,3</sup> · A. Grytsan<sup>3</sup> · Y. Loh<sup>4,5</sup> · P. A. Brouwer<sup>6</sup> · T. Andersson<sup>6,7</sup> · Namrata Gundiah<sup>8</sup> · Anne M. Robertson<sup>9</sup> · Paul N. Watton<sup>2,3,9</sup> · Michael Söderman<sup>6</sup>

Received: 9 July 2018 / Accepted: 8 March 2019 / Published online: 26 March 2019  
© Springer-Verlag GmbH Germany, part of Springer Nature 2019

### Abstract

**Background** Cerebral vasospasm (CVS) following subarachnoid hemorrhage occurs in up to 70% of patients. Recently, stents have been used to successfully treat CVS. This implies that the force required to expand spastic vessels and resolve vasospasm is lower than previously thought.

**Objective** We develop a mechanistic model of the spastic arterial wall to provide insight into CVS and predict the forces required to treat it.

**Material and Methods** The arterial wall is modelled as a cylindrical membrane using a constrained mixture theory that accounts for the mechanical roles of elastin, collagen and vascular smooth muscle cells (VSMC). We model the pressure diameter curve prior to CVS and predict how it changes following CVS. We propose a stretch-based damage criterion for VSMC and evaluate if several commercially available stents are able to resolve vasospasm.

**Results** The model predicts that dilatation of VSMCs beyond a threshold of mechanical failure is sufficient to resolve CVS without damage to the underlying extracellular matrix. Consistent with recent clinical observations, our model predicts that existing stents have the potential to provide sufficient outward force to successfully treat CVS and that success will be dependent on an appropriate match between stent and vessel.

**Conclusion** Mathematical models of CVS can provide insights into biological mechanisms and explore treatment approaches. Improved understanding of the underlying mechanistic processes governing CVS and its mechanical treatment may assist in the development of dedicated stents.

**Keywords** Vasospasm · Stent · Stentplasty · Mathematical modeling · Vascular smooth muscle cells

### Abbreviations

$p_{\text{sys}}$	Systolic pressure (value: 16 kPa)	$k_E$	Material parameter elastin (value: 93.14 kPa)
$H/R$	Ratio of unloaded thickness to unloaded radius (value: 0.2)	$k_M^{\text{pass}}$	Material parameter VSMC (passive) (value: 22.09 kPa)
$\lambda_z$	Axial stretch (value: 1.3)	$k_M^{\text{act}}$	Material parameter VSMC (active) (value: 18.07 kPa)

✉ P. Bhogal  
bhogalweb@aol.com

<sup>1</sup> Department of Interventional Neuroradiology, The Royal London Hospital, Whitechapel Road, London, E1 1BB, UK

<sup>2</sup> Department of Computer Science, University of Sheffield, Sheffield, UK

<sup>3</sup> Insigneo Institute for in silico Medicine, University of Sheffield, Sheffield, UK

<sup>4</sup> Uniformed Services University, University of California, Los Angeles, USA

<sup>5</sup> Swedish Neuroscience Institute, 550 17th Avenue Seattle, Washington, 98122, USA

<sup>6</sup> The Karolinska University Hospital, 171 76 Stockholm, Sweden

<sup>7</sup> AZ Groeninge, Kortrijk, Belgium

<sup>8</sup> Department of Mechanical Engineering, Indian Institute of Science, Bangalore, India

<sup>9</sup> Department of Mechanical Engineering and Materials Science, University of Pittsburgh, Pittsburgh, PA, USA

$k_{C_M}$	Material parameter medial collagen (value: 639.5 kPa)
$k_{C_A}$	Material parameter for adventitial collagen (value: 5115.6 kPa)
$f_P$	Passive stiffness factor (before vasospasm) (Value: 1)
$f_a$	Active stiffness factor (before vasospasm) (value: 1)
$\lambda_M^{\text{mean}}$	Cell stretch at which VSMC active response is maximal (value: 1.1)
$\lambda_M^{\text{max}}$	Maximum cell stretch at which VSMC's active response is zero (value: 1.8)
$\lambda_{M_{AT}}$	VSMC attachment stretch (value: 1.15)
$\lambda_{C_M}^{\text{max}}$	Maximum medial collagen fiber attachment stretch (value: 1.07)
$\lambda_{C_M}^{\text{min}}$	Minimum medial collagen fiber attachment stretch (value: 1.0)
$\lambda_{C_A}^{\text{max}}$	Maximum adventitial collagen fiber attachment stretch (value: 1.0)
$\lambda_{C_A}^{\text{min}}$	Minimum adventitial collagen fiber attachment stretch (value: 0.8)

## Introduction

Balloon angioplasty is a recognized treatment option for patients with delayed cerebral vasospasm (CVS) secondary to subarachnoid hemorrhage (SAH); however, the exact mechanism by which angioplasty results in long lasting vasodilatation remains unknown. Honma et al. [1] suggested that the mechanism of action of balloon angioplasty involves the disruption of both the degenerative muscle and the proliferative non-muscle components, mainly in the media of the vasospastic vessels. Indeed, it is generally believed that, in order for balloon angioplasty to resolve CVS, damage to the underlying collagenous extracellular matrix (ECM) is required [2]; however, there are many studies that have demonstrated resolution of vasospasm but without evidence of damage to the underlying ECM [3–6]. Therefore, the results of previous work have not provided a conclusive answer to the question of whether disruption of the ECM is required in order to achieve long lasting vasodilatation.

In recent previous publications [7, 8], several members of this group documented their initial experience with the use of stent-retrievers to treat medically refractory symptomatic CVS, so-called stentplasty. It was noted that stents can resolve CVS; however, the efficacy is variable with more consistent vasodilatation seen in smaller arteries such as the M2 and A2 branches. Given that these stents provide an outward pressure (approx. 0–23 kPa, depending on model and diameter, see Appendix C) which is up to an order of magnitude lower than balloon angioplasty (up to 300 kPa [2]), our experience seems at odds with the com-

monly held belief that damage to the ECM is necessary to resolve CVS.

The variability in the effectiveness of stents points to the need for a mechanistic understanding of the effects of these stents in order to guide future treatment. Differences in outcome are conjectured to be dependent on the outward force exerted by the stents and their ability or lack thereof to reach a dilatation threshold, i.e. a critical diameter beyond which a stent must expand the artery in order to successfully resolve vasospasm. This raises the questions: what determines the dilatation threshold of an artery in vasospasm? Can we predict whether a stent will be successful in resolving the disease (i.e. expanding the artery beyond the dilatation threshold)?

In this article, we propose a mathematical model focused on the mechanobiology of soft tissue with the aim of providing insight into the mechanism of action behind the mechanical treatment of CVS. In particular, our model captures the changing roles of the active and passive vascular smooth muscle cells following CVS and after treatment with stents. The work ends with a comparison of the success of currently available stents for treating vasospasm. Our model predictions are consistent with our recent clinical observations that it is not necessary to damage the ECM to successfully treat CVS.


## Methods

We introduce a mathematical model for a cerebral artery and use this to describe its pressure-diameter (p-d) curve and predict how this curve changes following CVS. Assuming a stretch-based damage criterion for vascular smooth muscle cells (VSMCs), this allows us to estimate the (minimum) pressure an interventional device needs to apply to the vessel wall to resolve CVS.

### Mathematical Model of the Arterial Wall: Prevasospasm

We utilize existing mathematical approaches which model the arterial tissue as a constrained mixture [9, 10] and attribute its load bearing to the distinct contributions from elastin [11], distributions of collagen fibers [12–14] and VSMCs [15]. Here we overview the key features that the mathematical model captures; further details are provided in Appendix A for the interested reader.

The Law of Laplace is a simple force balance on a vessel, which when applied to an elastic cylinder model of an artery relates the transmural pressure  $p$  to the deformed

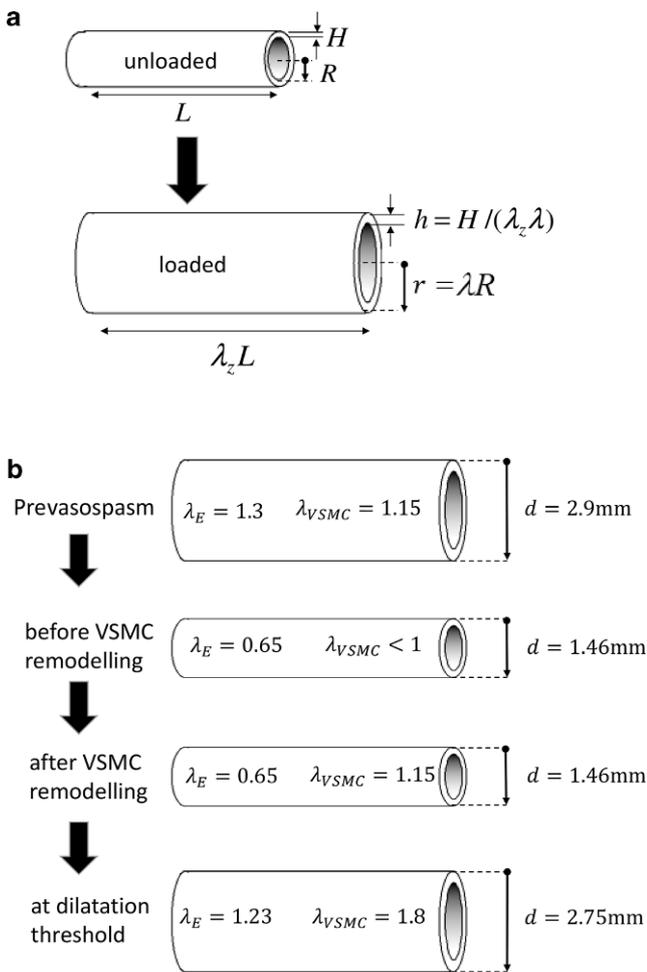

**Fig. 1** **a** The arterial geometry is approximated as a nonlinear elastic cylinder with unloaded radius  $R$  and thickness  $H$ , which is pressurized and axially prestretched to mimic in vivo conditions. **b** Diameters, internal pressures and constituent stretches at different phases of our model of vasospasm. In the prevasospasm phase, arterial diameter at systolic blood pressure is 2.9mm, VSMC stretch equals its attachment stretch. In the early phase of vasospasm, the constriction is chemically driven and VSMCs have not yet remodeled. Following remodeling, VSMCs have returned to their attachment stretch while elastin has not remodeled so its stretch has not changed. Finally, if a stent provides enough pressure to exceed a critical value, a dilatation threshold is reached at which VSMCs are brought to mechanical failure and incapacity to bear the pressure load. This signifies successful treatment of CVS. (VSMC vascular smooth muscle cells, CVS cerebral vasospasm)

wall thickness  $h$ , the diameter  $d$  and the circumferential intramural stress  $\sigma$  as follows (Fig. 1a):

$$p = \frac{2h\sigma}{d} \tag{1}$$

This law is useful to capture aspects of the mechanical behavior of the whole wall, but it does not capture its layered structure or describe how the individual constituents contribute to bearing the pressure load; however, with a sub-

tle sophistication, we can write a modified Law of Laplace as:

$$p = \frac{2h}{d} (\sigma_E + \sigma_{CM} + \sigma_{CA} + \sigma_{VSMCp} + \sigma_{VSMCa}), \tag{2}$$

where the wall stress  $\sigma$  is additively split into the stress contributions from the individual load bearing constituents of the arterial wall: elastin, medial and adventitial collagen, and passive and active VSMC; these are denoted  $\sigma_E, \sigma_{CM}, \sigma_{CA}, \sigma_{VSMCp}$  and  $\sigma_{VSMCa}$ , respectively.

Of great importance for the normal functioning of the arterial wall is that at a given expanded state of the artery, these wall components experience different stretches from one another. This is possible because they are manufactured (produced and configured) with different physical conformations, dependent on their mechanical role. Hence, we model the stress responses as functions of the stretches that individual constituents experience. We can represent this dependence mathematically for each wall component as:

$$\begin{aligned} \sigma_E &= \sigma_E(\lambda_E); \sigma_{CM} = \sigma_{CM}(\lambda_{CM}); \\ \sigma_{CA} &= \sigma_{CA}(\lambda_{CA}); \\ \sigma_{VSMCp} &= \sigma_{VSMCp}(\lambda_{VSMC}); \sigma_{VSMCa} = \sigma_{VSMCa}(\lambda_{VSMC}) \end{aligned} \tag{3}$$

where  $\lambda_E, \lambda_{CM}, \lambda_{CA}, \lambda_{VSMC}$  denote the circumferential stretches of elastin, medial and adventitial collagen and VSMCs. The stretch for each component is defined as the current length of the component divided by its unloaded length. Hence, for example, when a medial collagen fiber is not stretched,  $\lambda_{CM}=1$  and when the artery further expands, the fiber will also stretch so that  $\lambda_{CM}>1$ . It is understood in Eq. 2 that a passive wall component will not experience stress until it is stretched (e.g.  $\sigma_{CM}=0$ , until  $\lambda_{CM}>1$ ).

We assume constituents are integrated into the arterial wall in the loaded configuration with a preferred stretch, which we refer to as the attachment stretch [9]. For example, we model VSMCs to have an attachment stretch of 1.15 at systolic pressure (Fig. 1b). The choice of attachment stretches for adventitial and medial collagen are motivated by the experimental observations [13, 16] that:

1. medial collagen contributes to load bearing in homeostatic configuration whilst adventitial collagen acts as a protective sheath,
2. both medial and adventitial collagen appear with different levels of waviness and are thus recruited to load bearing at different stretches (i.e. wavier fibers at higher stretches).

In order to capture these features, in the systolic configuration: medial collagen fibers are prescribed to have attachment stretches ranging from 1 to 1.07 (thus all fibers of the distribution are bearing load); adventitial collagen fibers are prescribed to have attachment stretches between

0.8 and 1 (thus no fibers are mechanically engaged until the vessel is enlarged further).

In summary, this modelling approach enables us to:

- account for how the total mechanical behavior of the artery relates to the mechanical response (and stretches) of its individual constituents,
- predict how changes in quantity (growth) and organization (remodeling) of these constituents during healthy adaptation, aging and disease affect the mechanical behavior of the wall,
- predict how damage to these constituents affects the mechanical function of the artery, for example after treatment with stents or balloon angioplasty.

## Results

### Mechanical Model of Arterial Wall


The pressure-diameter (p-d) curve for our model of a healthy cerebral artery is shown in Fig. 2. It depicts how the wall components (constituents) contribute to the overall load bearing of the arterial wall. At systolic pressure (16 kPa), the arterial diameter is 2.9 mm (indicated by red dashes) and it can be seen that the p-d curve (solid curve) is the sum of the p-d curves of the individual constituents (non-solid). In essence, this figure illustrates the contributions of each wall component to support the transmural pressure:

$$p = p_E + p_{CM} + p_{CA} + p_{VSMCp} + p_{VSMCa},$$

which is obtained simply from Eq. 2 by using the relationship between pressure and stress for each component, e.g.  $p_E = 2h\sigma_E/d$  and analogously for the other terms, consistent with (1). Note, the implications of distinct constituent attachment stretches are visible in Fig. 2 where it can be seen that the individual wall components begin to be recruited to load bearing at different arterial diameters (elastin at ~1.95 mm, VSMCs at ~2.25 mm and collagen at ~2.65 mm).

### Mechanical Model of Arterial Wall: Postvasospasm

Based on reports in the literature, we model CVS in the following manner. At the onset of vasospasm, the VSMCs contract and as a result the diameter at systolic pressure is decreased (Fig. 1b); for purposes of illustration, we simulate a 50% reduction in systolic diameter so that the arterial diameter at systolic pressure is reduced to 1.46 mm. Following this initial constriction, the following changes are conjectured to occur over a time scale on the order of days

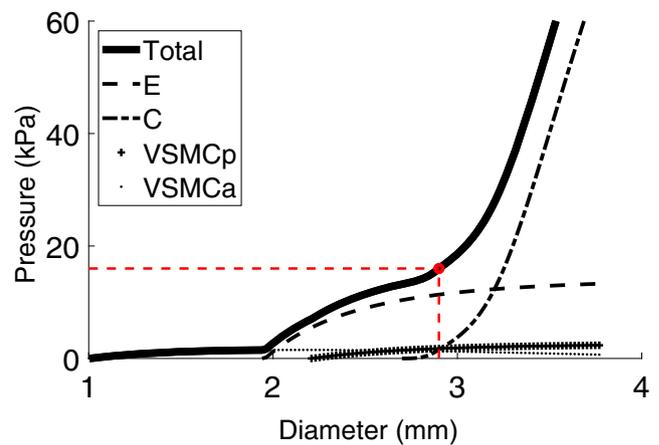

**Fig. 2** Pressure-diameter curve for a middle cerebral artery (*solid curve*). Physiological systolic blood pressure of 16 kPa corresponds to healthy diameter of 2.9 mm (*red dashed lines*). The non-solid curves represent the contributions of the individual load-bearing constituents: elastin, collagen (medial+adventitial), passive response of VSMCs and active response of VSMCs


to weeks (much larger than the cardiac cycle) whilst the diameter is maintained:

- VSMCs remodel to restore their stretch towards their preferred value (VSMC attachment stretch) on the vasospastic vessel (via remodeling [9, 10]: this is achieved through reconfiguration of their internal cytoskeleton and/or of their attachments to the ECM [17, 18]).
- As VSMCs remodel their stretch, to maintain force balance, VSMCs' cell stiffness increases, captured by increasing material parameters of  $\sigma_{VSMCp}$  and  $\sigma_{VSMCa}$  [18, 19].
- Extracellular matrix components (elastin and collagen) do not remodel; elastin production ceases after puberty and we assume collagen turnover rate is long compared to the time scale of CVS.


These model features enable us to predict how the p-d curve is altered by CVS (Fig. 3). For our illustrative example, we prescribed increases of material parameters for  $\sigma_{VSMCp}$  and  $\sigma_{VSMCa}$  by 20% and 47.5%, respectively (we refer to Appendix B for more details and a parameter study). Note that the loading curves for the VSMCs have shifted to the left (to maintain VSMC attachment stretch) and upwards (increased stiffness of VSMC to maintain mechanical equilibrium at systolic pressure). The solid line reflects the additive effect of these changes on the total response of the wall; note, given that we assume elastin and collagen do not remodel, their curves do not change.

### Damaging the Arterial Wall: Dilatation Threshold

Our model explicitly represents the stretches of the individual constituents and thus we can explicitly define damage

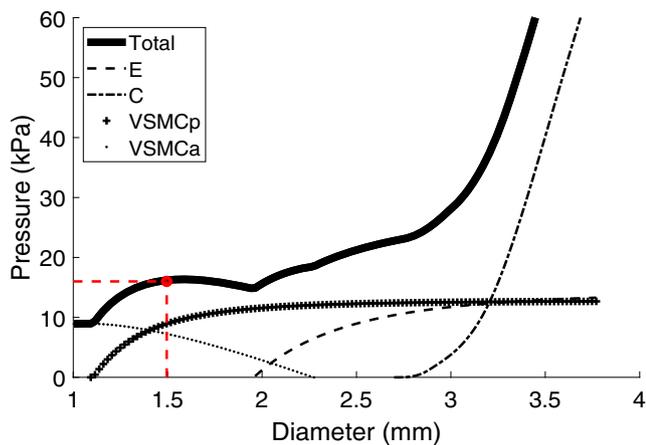

**Fig. 3** Pressure-diameter curve for a vasospastic middle cerebral artery with original systolic diameter 2.9mm that contracted to a systolic diameter of 1.46mm. The *non-solid curves* represent the contributions of the individual load-bearing constituents

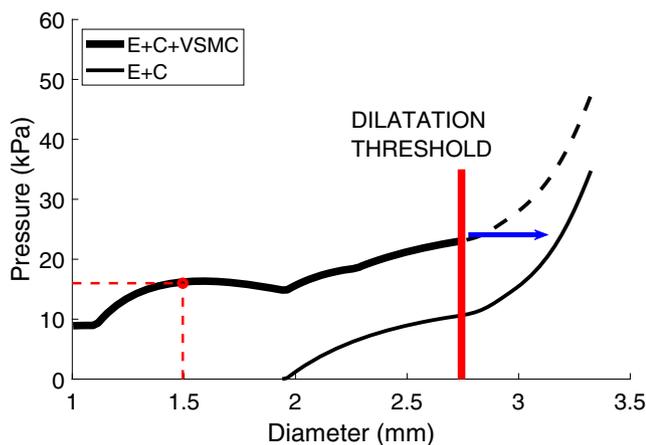

**Fig. 4** Pressure-diameter curve for the vasospastic artery before and after VSMC damage. When the dilatation threshold is reached, VSMCs cease to contribute to load bearing and only elastin and collagen are bearing the pressure load (*thinner solid curve*)

criteria for each constituent; where by damage we mean cessation of mechanical contribution to load bearing. The VSMC damage could arise from either rupture of the cell’s internal cytoskeleton or cell detachment from the ECM or both.

We define a clinically relevant dilatation threshold as the critical stretch at which VSMCs are damaged. Here, we assume that once the VSMCs are damaged, they not only cease to contribute to load bearing but also no longer generate active tension. Hence, if a stent can provide sufficient outward pressure to expand the artery beyond the dilatation threshold, CVS is successfully treated. A reasonable upper bound for the critical VSMC stretch is 1.8 [20]. Given that we assume VSMCs have a stretch of 1.15 in the post-vasospasm state (1.46mm diameter for this illus-

trative model), this implies a dilatation threshold diameter of 2.75 mm (Fig. 1b).

We predict that a stent will be successful in treating CVS if the total pressure that is exerted on the arterial wall (sum of blood pressure plus stent pressure) remains above the p-d curve for the artery (solid curve) up until the dilatation threshold is reached: the biomechanical explanation of this being that the stent is applying enough force onto the vessel wall to expand it until VSMCs are damaged. For this illustrative example, it can be seen that the sum of the pressure provided by the stent plus the systolic blood pressure must exceed 23 kPa at the dilatation threshold diameter to treat the vasospasm. Hence, for a systolic blood pressure of 16kPa, this implies a stent would need to provide at least an additional 7kPa of pressure to the arterial wall up to a diameter of 2.75 mm.

Observe that the dilatation threshold is slightly lower than the original vessel diameter at systolic pressure and thus the collagen and elastin fibers are not damaged. Therefore, once the dilatation threshold is reached, the pressure relationship (2) becomes, (Fig. 4),


$$p = \frac{2h}{d} (\sigma_E + \sigma_{CM} + \sigma_{CA}). \tag{4}$$

### Modelling Treatment of Vasospasm

We now apply our mechanistic model to test whether a given stent would provide sufficient force to dilate the vessel beyond the dilatation threshold and thus resolve CVS. To do this, we first convert the chronic outward force data available for commercial stents into stent pressures (see Appendix C), [21]. An important observation to make about the mechanics of stents is that the pressure they exert on the wall decreases as they unfold to larger diameters (Appendix C, Figs. C.1 and C.2), in contrast to the mechanics of balloon angioplasty.

Fig. 5 illustrates how the total pressure curve (systolic blood pressure + stent pressure) of two example stents, Solitaire (Medtronic, Dublin, Ireland) 6 mm and Trevo (Stryker, Fremont, CA, USA) 4 mm, is related to their deployed diameter. The p-d curve (solid curve, Fig. 5) is the same as the one given in Figs. 3 and 4 and provides information about which diameter corresponds to which internal pressure, in this case for a vasospastic middle cerebral artery at 50% stenosis.

As seen in Fig. 5, the Solitaire 6mm stent can apply more than sufficient pressure to dilate the stenosed vessel above the dilatation threshold. In contrast, the Trevo 4 mm can only dilate the vessel a few millimetres before a new mechanical equilibrium is reached at a diameter (point E) lower than the dilatation threshold. The thinner solid line shows the mechanical response curve for the vessel after

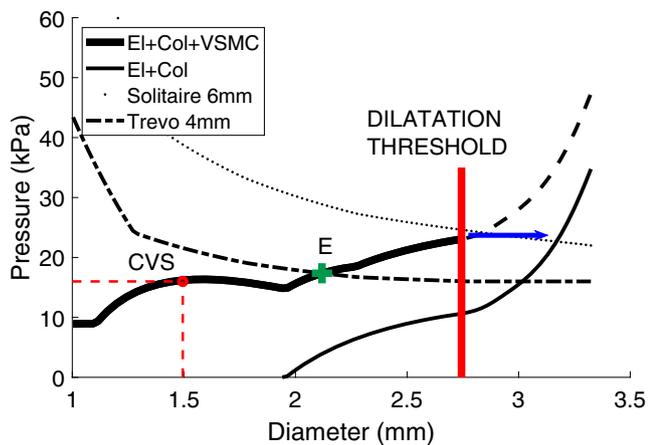

**Fig. 5** Effectiveness of two stent-retrievers in resolving vasospasm in a middle cerebral artery with 50% stenosis. The stent is effective if its related curve remains above the solid curve up until the dilatation threshold. In this example, Solitaire 6mm would be successful, whereas Trevo 4mm (4 × 20 mm) would not because mechanical equilibrium would be reached at point E, which is well before the dilatation threshold

treatment with the Solitaire 6 mm, i.e. following damage to VSMCs and having only elastin and collagen contributing to load bearing: the diameter at systole has increased from 1.46 mm (vasospastic) to 3.2 mm. Note that the initial systolic diameter prior to CVS was 2.9 mm (Fig. 2). Next, we model arteries of several different representative diameters (1.5, 2, 2.9 and 4 mm) at 50% stenosis and simulate treatment with the following stents: Solitaire 6 mm (Covidien), Solitaire 4 mm (Covidien), Capture 3 mm (Mindframe), Trevo 4 mm (Stryker). It can be seen that all stents are effective in resolving CVS for the smaller arteries whilst none are successful for the larger arteries (Fig. 6); however, even when the stents fail to resolve CVS, notice that the magnitude of pressure necessary to resolve the disease is much smaller than the maximum possible pressure exerted by balloon angioplasty (300 KPa). Hence, our model predicts that stronger stents would be able to overcome the dilatation threshold and treat CVS with limited risk of damage to the underlying ECM.

## Discussion


Previous clinical results from our group have demonstrated the tremendous potential of vascular stents in treating vasospasm of cerebral vessels; however, the success has been uneven so far, thus pointing to the need for a mechanistic understanding of changes to the arterial wall during stent deployment in vasospastic arteries. In this paper we present a mathematical model for this process, which demonstrates that the substantially lower forces generated by properly chosen stents compared with balloon angioplasty, can effec-

tively treat vasospasm by altering the VSMCs, even without damage to the ECM.

We believe the importance of the mathematical model is its accurate replication of our clinical experience regarding the use of stents to treat CVS following subarachnoid hemorrhage. Whilst we have seen good results in smaller vessels, such as spastic M2 and A2 branches, we have seen mixed results in the M1 segment and we are yet to see a successful dilatation of the terminal internal carotid artery (ICA). Based on the current studies, we believe that this is due to a lack of sufficient outward radial force exerted by the existing stents, which have been designed for a different task, i.e. to perform mechanical thrombectomy in acute thromboembolic stroke. In particular, consistent with these recent clinical observations, the model predicts that stents provide sufficient outward force to treat small diameter arteries but may not provide sufficient force with larger diameter arteries. Hence, specifically designed stents may offer a viable alternative to balloon angioplasty for the mechanical resolution of CVS. The advantages of such treatment (over angioplasty) include a lower risk of damage to the ECM and thus a decrease in the risk of rupture of the arterial wall.

In this modelling approach, we assume that the resolution of CVS is achieved by disrupting the VSMCs sufficiently to eliminate their contribution to load bearing. The model predicts that damage to the matrix is not a prerequisite for successful mechanical treatment of CVS. This is supported by other observations in the literature. For example, Kobayashi et al. [3] studied vasospastic primate cerebral arteries that were successfully treated with angioplasty and did not report any significant ECM damage. Similarly, Macdonald et al. [4] have shown in a rabbit model that successful angioplasty resulted in damage to the VSMCs but not the ECM.

A key assumption in this work is the existence of a dilatation threshold that once reached renders the VSMC unable to generate vasoconstriction. It is hypothesized that this level is associated with the VSMCs being detached from the ECM and/or having their stress fibers ruptured. Furthermore, it is assumed that this threshold is too low to damage collagen and elastin fibers. This assumption is supported by experimental observations. Chan et al.'s [5] in vitro study of vasospastic canine basilar arteries assessed the arteries both morphologically and pharmacologically: in congruence to Kobayashi et al. [3] and MacDonald et al. [4], they observed no difference between the ECM collagen fibers and elastin even in vasospastic vessels that were subjected to balloon angioplasty compared to those that were not, i.e. they saw no fiber breakage following balloon angioplasty. Hence, this suggests that no damage would be expected at the much lower loads achieved during stent deployment. Interestingly, they observed that the response

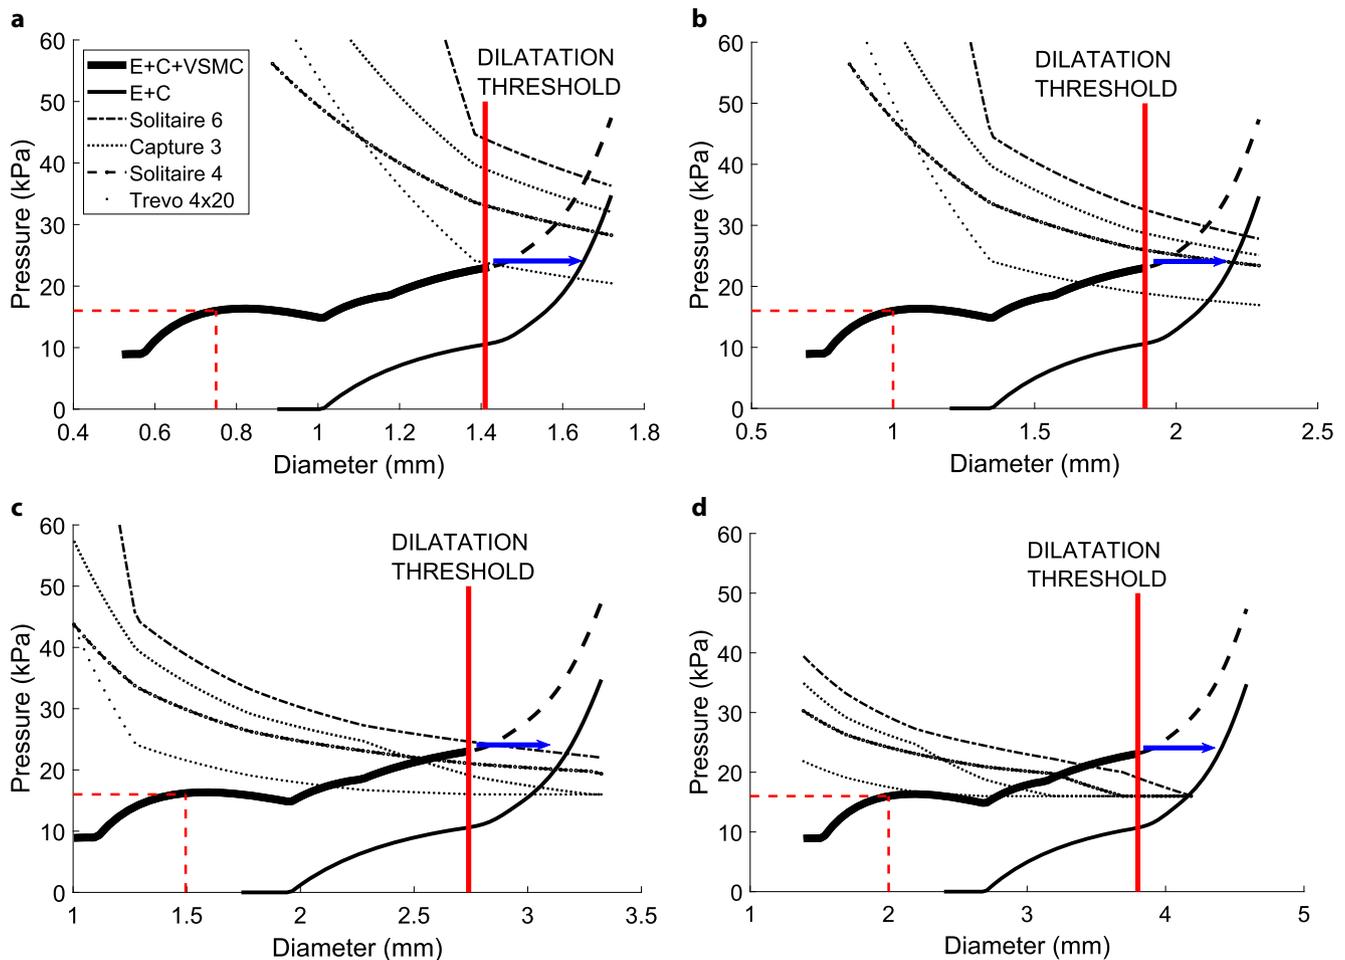

**Fig. 6** Effectiveness of four stent-retrievers in vasospastic arteries of physiological diameters 1.5 mm (a), 2 mm (b), 2.9 mm (c) and 4 mm (d), at 50% stenosis. In the 1.5 mm artery all the stents expand the wall beyond the dilatation threshold. In the 4 mm artery, they open the artery to new diameters, which are less than the dilatation threshold and are therefore not effective in treating vasospasm

of both normal, non-spastic vessels and vasospastic vessels to vasoconstricting substances following balloon angioplasty was significantly decreased. Macdonald et al. [6] also demonstrated a similar decrease in constriction following balloon angioplasty and they proposed that balloon angioplasty somehow decreases the contractility of VSMCs. It remains to assess changes in vasoconstriction response during the much lower loads associated with stent deployment. The paralysis and loss of contractility of VSMCs has been observed in experimental dilatation studies of peripheral arteries [22–25]; however, the exact cellular and/or intracellular mechanism has not yet been determined and more experimental studies on the problem are advised.

In 1990, Fischell et al. [20] observed that following balloon angioplasty in both relaxed and contracted arteries, an arterial paralysis was seen, but that this did not have a relationship with prolonged balloon inflation. They demonstrated that the same degree of balloon dilatation in relaxed vessels produced significantly less, if any, arterial paralysis compared to contracted vessels. Therefore, we con-

jecture that contraction of VSMCs predisposes them to arterial paralysis when subjected to stretch and balloon angioplasty. This may help explain the frequent finding of arterial paralysis seen in spasm-prone rabbit arteries *in vivo* [25–28]. The question remains, though, as to why contraction of the VSMCs predisposes them to arterial paralysis following angioplasty: is it due to breakage of the VSMCs' internal contractile cytoskeleton, could it be associated with their detachment from the ECM or is it a combination of both? Either way, they will no longer contribute to the bearing of the pressure load nor will they be able to contract and cause the spasm to return.

We believe that one of the most important points of our work is that the success of mechanical dilatation appears to be related to the degree of contraction. According to our model, deployment of the stent is more likely to result in successful dilatation if the vessel is contracted and therefore arterial relaxation with vasodilators prior to stentplasty should not be performed. Kwon et al. [29], in their retrospective clinical analysis, demonstrated a 60% recurrence

of vasospasm if nicardipine was infused prior to stentplasty compared to 0% recurrence of vasospasm if stentplasty was performed prior to nicardipine infusion.

The mathematical model presented is a conceptual representation of the mechanics of the arterial wall, CVS and its treatment. It has many simplifications and does not represent the full biological complexity of the arterial wall. For instance, we model mechanics of the arterial wall using a thin wall assumption. This hypothesis requires that the strain perceived by the constituents in the arterial wall is constant throughout its thickness. While this holds true for a healthy artery, radial gradients may be important following vasospasm. Additional studies using a thick-walled model [30] and guided by additional experiments can be performed. Another limitation is the assumption that collagen does not remodel following vasospasm. This choice is motivated by the long half-life of the collagen fiber (about 72 days) compared to the time scale of vasospasm. Nevertheless, it is straightforward to include partial remodeling in a more sophisticated version of the present model.

We assume that the stiffness of VSMCs increases in the vasospastic state. This is consistent with the observation that VSMC remodeling of the cytoskeleton modulates the cell stiffness and contractility through signaling pathways; increased cell stiffness leads to an increase in the overall vascular stiffness [31]; however, it is unclear how this increase in stiffness is apportioned between the passive and active stress contributions. In the absence of *in vitro* or *in vivo* data to inform the modelling, a parametric study was run (details in Appendix B) covering the range of possible combinations of active and passive stress contributions. These studies showed that the minimum amount of pressure a stent needs to mechanically resolve vasospasm varied between 5 and 11 kPa, as a result of this uncertainty in load proportioning. Even with this variability, the general conclusion still holds, *i.e.* that the applied pressure required for a stent to resolve CVS is an order of magnitude lower than that provided by balloon angioplasty; however, this parameter study highlights the need for continued data-driven studies to improve our understanding of the mechanobiology of VSMCs in the spastic artery.

The mathematical model provides insight into the underlying mechanisms of vasospasm and its resolution; however, it incorporates a simplified representation of the mechanics, biology and mechanobiology of the arterial wall and there is a need for *in vivo/in vitro* experiments to quantify model parameters and evaluate the consistency of modelling hypotheses. In particular, experimental guidance is needed to quantify how remodeling of the SMC influences their passive and active stress responses and how resolution of vasospasm is related to disruption of the VSMC cytoskeleton and/or attachment to the ECM. *In vitro* experimental investigations on individual cells combined with investigation of

tissue samples obtained from animal models of vasospasm will guide the development of more sophisticated mathematical models with improved predictive abilities.

Despite its relative simplicity, the authors believe the current model contains the essential features needed to guide future experiments on the pathophysiology and improved treatment of vasospasm. Understanding the biomechanical mechanisms of CVS would seem to be essential for designing improved therapeutic and interventional treatment options.

## Conclusion

Improved understanding of the underlying mechanistic processes governing CVS and its mechanical treatment may assist in the development of dedicated stents. The model presented here supports our clinical experience that currently available stents can successfully resolve CVS in smaller arteries but not in larger, more proximal arteries. The development of dedicated stents targeted to damaging VSMC in a larger range of cerebral arteries may provide a viable, reproducible and safe treatment option to treat delayed CVS.

**Funding** G. Pederzani is a PhD student of SoftMech, an EPSRC center for soft tissue mechanics and is funded by a PhD scholarship provided by the Department of Computer Science, University of Sheffield. P. Watton acknowledges partial support towards this work from SoftMech, UK EPSRC (EP/N014642/1).

**Author Contribution** P. Bhogal developed the theory. N. Gundiah advised on cell mechanobiology. G. Pederzani, A. Grytsan, A.M. Robertson and P.N. Watton developed the mathematical model. All authors contributed to the editing and reviewing of the paper. M. Söderman is guarantor.


## Compliance with ethical guidelines

**Conflict of interest** P. Bhogal is co-developer and co-patent holder of the Lumenate Stent and consults for Phenox. G. Pederzani, A. Grytsan, N. Gundiah, A.M. Robertson & P.N. Watton have no conflicts of interest. Y. Loh is a consultant for Balt, Neurvana and Medtronic. P. Brouwer is a consultant for Stryker, Medtronic and Cerenovus/Neuravi. T. Andersson is a consultant for Stryker, Covidien, Neuravi, Rapid Medical. M. Söderman is a consultant for Blockade, Neuravi, co-developer and co-patent holder of the Lumenate Stent.

**Ethical standards** For this article no studies with human participants or animals were performed by any of the authors. All studies performed were in accordance with the ethical standards indicated in each case. For this type of study formal consent is not required.

## Appendix A

The arterial wall is modelled as a nonlinear elastic cylindrical membrane [10] with thickness  $H$  and radius  $R$  in its unloaded configuration. *In vivo*, it is subject to an internal

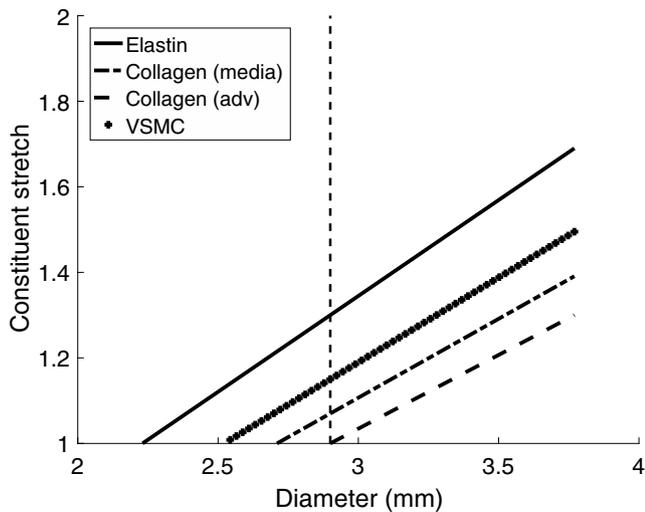

**Fig. A.1** Constituent stretch vs. diameter relationship for elastin, medial collagen, adventitial collagen and VSMCs. Given the different mechanical roles, constituents begin to bear the pressure load at different diameters and are configured at different stretches at the physiological diameter (vertical dashed line)

pressure  $p$  and axial stretch  $\lambda_z$ . The governing equation describing the balance of forces for mechanical equilibrium is:

$$p = \frac{h\sigma}{r}$$

Where the deformed radius  $r$  is given by  $r = \lambda R$  with  $\lambda$  the circumferential tissue stretch, the deformed thickness of the arterial wall is  $h = H/\lambda_z\lambda$ , and  $\sigma$  denotes the circumferential Cauchy stress. The arterial wall constituents are modelled as a constrained mixture, so that the total

(Cauchy) stress  $\sigma$  component for the arterial wall is the sum of stress contributions from the individual constituents, i. e.

$$\sigma = \sigma_E(\lambda) + \sigma_{CM}(\lambda_{CM}) + \sigma_{CA}(\lambda_{CA}) + \sigma_{VSMCp}(\lambda_M) + \sigma_{VSMCa}(\lambda_M)$$

where  $\sigma_E$ ,  $\sigma_{CM}$ ,  $\sigma_{CA}$ ,  $\sigma_{VSMCp}$  and  $\sigma_{VSMCa}$  denote the circumferential Cauchy stress contributions of elastin (E), medial collagen (CM), adventitial collagen (CA), passive and active VSMCs, respectively. We exclude the mechanical role of endothelial cells due to their negligible role in the mechanical behavior of the vessel [30].

We utilize a strain energy function for the collagen that accounts for the recruitment distribution of collagen fibers [13, 16]

$$\Psi_{C_J}(\lambda) = \int_1^\lambda \tilde{\Psi}_{C_J}(\lambda_{C_J}) \rho(\lambda_{R_J}) d\lambda_{R_J},$$

where the distribution of recruitment stretches  $\rho(\lambda_{R_J})$  is taken to be a triangular distribution function [12, 14] and the mechanical response of an individual fiber is linear, i. e.

$$\tilde{\Psi}_{C_J}(\lambda_{C_J}) = \frac{k_{C_J}}{2}(\lambda_{C_J} - 1)^2$$

Analytical expressions for the collagen Cauchy stresses [12] can then be obtained via,

$$\sigma_{C_J} = \lambda \frac{\partial}{\partial \lambda} \Psi_{C_J}(\lambda),$$

**Table A.1** Model parameters used for the simulations

Parameter	Meaning	Value
$p_{sys}$	Systolic pressure	16 kPa
$H/R$	Ratio of unloaded thickness to unloaded radius	0.2
$\lambda_z$	Axial stretch	1.3
$k_E$	Material parameter elastin	93.14 kPa
$k_M^{pass}$	Material parameter VSMC (passive)	22.09 kPa
$k_M^{act}$	Material parameter VSMC (active)	18.07 kPa
$k_{CM}$	Material parameter medial collagen	639.5 kPa
$k_{CA}$	Material parameter for adventitial collagen	5115.6 kPa
$f_p$	Passive stiffness factor (before vasospasm)	1
$f_a$	Active stiffness factor (before vasospasm)	1
$\lambda_M^{mean}$	Cell stretch at which VSMC's active response is maximal	1.1
$\lambda_M^{max}$	Maximum cell stretch at which VSMC's active response is zero	1.8
$\lambda_{MAT}$	VSMC attachment stretch	1.15
$\lambda_{CM}^{max}$	Maximum medial collagen fiber attachment stretch	1.07
$\lambda_{CM}^{min}$	Minimum medial collagen fiber attachment stretch	1.0
$\lambda_{CA}^{max}$	Maximum adventitial collagen fiber attachment stretch	1.0
$\lambda_{CA}^{min}$	Minimum adventitial collagen fiber attachment stretch	0.8

The mechanical responses of elastin and passive VSMCs are modelled using neo-Hookean constitutive models [9] and it follows that

$$\sigma_E = k_E \lambda^2 \left( 1 - \frac{1}{\lambda^2 \lambda^4} \right),$$

$$\sigma_{\text{VSMC}_p} = f_p k_M^{\text{pass}} \lambda_M^2 \left( 1 - \frac{1}{\lambda^2 \lambda_M^4} \right),$$

whilst the active response of VSMCs follows [31, 32]

$$\sigma_{\text{VSMC}_a} = f_a c_v k_M^{\text{act}} \lambda_M \left[ 1 - \left( \frac{\lambda_M^{\text{mean}} - \lambda_M}{\lambda_M^{\text{mean}} - \lambda_M^{\text{max}}} \right)^2 \right]$$

The material parameters  $k_E, k_M^{\text{pass}}, k_M^{\text{act}}, k_C$  are inferred by prescribing the proportion of load borne by the constituent in the initial homeostatic configuration [33–35]. We assume that at systolic pressure the stretch  $\lambda = 1.3$ , the elastin bears 70% of the load, passive VSMC bears 10% of the load, active VSMC bears 10% of the load medial collagen bears 10% of the load; adventitial collagen is unrecruited so doesn't bear any load. Note  $f_p, f_a$  are dimensionless parameters for increasing the passive and active stress responses following vasospasm to maintain mechanical equilibrium.

### Natural Reference Configurations

The mechanical responses are defined as functions of the stretches that individual constituents experience, i.e.

$$\lambda_J = \frac{\lambda}{\lambda_{R_J}},$$

where  $\lambda$  denotes the tissue stretch,  $\lambda_J$  denotes the stretches of medial and adventitial collagen ( $J = C_M, C_A$ ) and VSMC ( $J = S$ ); the recruitment stretches  $\lambda_{R_J}$  define the onset of load bearing (Fig. A.1).

Initial values for recruitment stretches are obtained by prescribing the attachment stretches of constituents (or VSMC) in the (prevasospasm) loaded configuration, i.e.

$$\lambda_{R_J} = \frac{\lambda}{\lambda_J} \Big|_{p_{\text{sys}}, \lambda_z}$$

For collagen, each (symmetric) triangular distribution of fibers requires specification of maximum/minimum fiber attachment stretches, i.e.  $\lambda_{C_J}^{\text{max}}$  and  $\lambda_{C_J}^{\text{min}}$ , respectively. We model distinct distributions so that medial collagen bears load in homeostatic configuration, while adventitial collagen is modelled as playing a purely protective role, i.e. begins to bear load after systole.

## Appendix B

In vasospasm, the contraction of the VSMC reduces the vessel cross-section, removing load from the ECM components as the stretch of these components drops below one. As a result, the VSMC must bear all of the load, albeit at a smaller diameter. We assume that in the time between vasospasm onset and treatment the mechanical contribution from collagen and elastin remains negligible in comparison to the VSMC contributions (despite possible remodeling of collagen fibers). Although the VSMCs must bear the entire transmural load, the relative contributions of the active and passive components may shift in time. The degree and timing of this shift will depend on a number of factors involving the damage to the VSMC during treatment as well as the VSMC remodeling process for the individual patient. In this Appendix, we do not directly model these changes, but rather perform a parametric study to conservatively explore the possible impact that the largest possible variation in relative load bearing would have on predicted stent requirements.

In the parametric study, the relative roles of active and passive VSMC are controlled by varying parameters  $f_p$  and  $f_a$  (see Discussion for a biological interpretation of these changes). Both parameters are greater than or equal to 1 and are coupled in that their combined influence maintains equilibrium of the vessel. In the main body of the text, a specific case ( $f_p = 1.2, f_a = 1.475$ ) was considered. Here results are obtained over the entire parameter space. To do so, we first obtained the solutions for the two extreme cases with  $f_p = 1$ , and  $f_a = 1$ , respectively. In particular, if the passive response is not affected ( $f_p = 1$ ), then  $f_a$  must increase by 75%; conversely, if  $f_a = 1$ , then  $f_p$  increases by 55%, Fig. B.1. We then gradually increased  $f_p$  from 1 to 1.55 (with  $f_p = 1.55$  corresponding to  $f_a = 1$ ) by small constant increments and solved the equation of mechanical



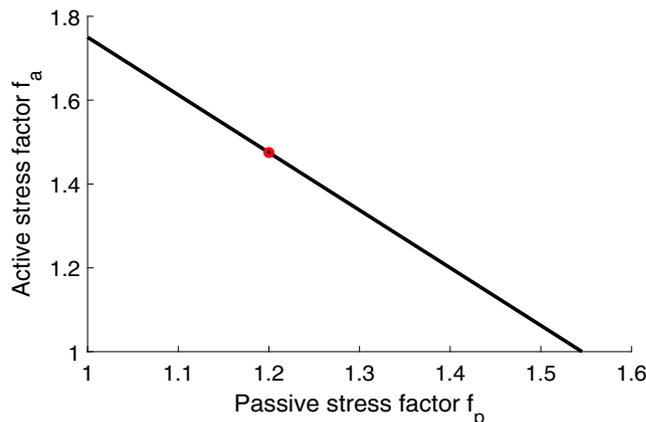



Fig. B.1 Plot of the parameter pairs  $f_a$  vs  $f_p$  that solve mechanical equilibrium for a vasospastic middle cerebral artery at 50% stenosis. The represented values cover all possible solutions

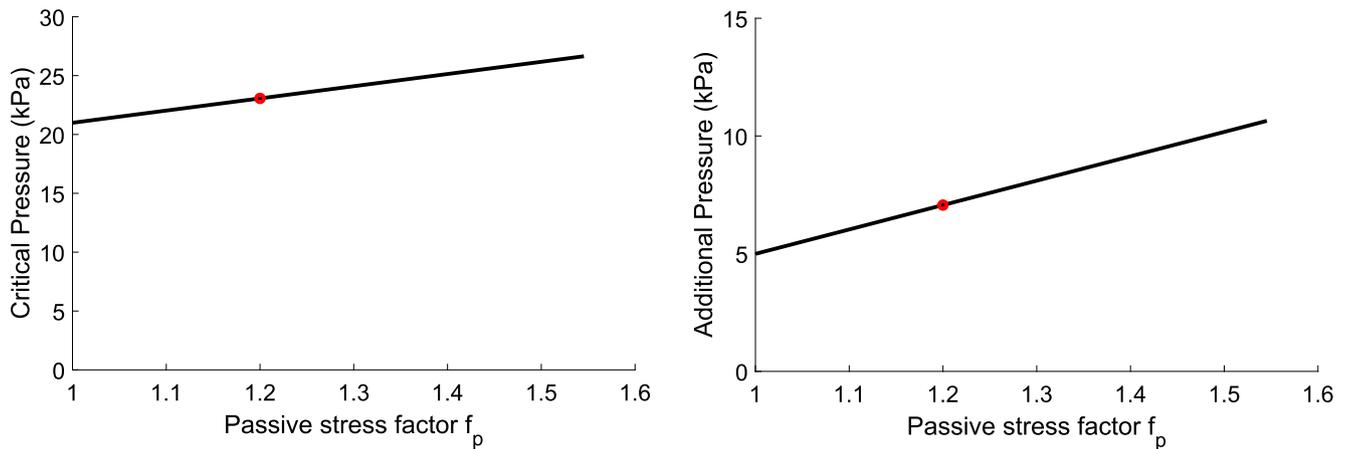

**Fig. B.2** Plot of the critical pressure (*above*) and additional pressure (*below*) vs. increase in passive response in vasospasm at 50% stenosis. The critical pressure is defined as the amount of pressure necessary to be applied to the arterial wall to reach the dilatation threshold, while the additional pressure is the amount of pressure an interventional device should provide to reach such dilatation threshold. Equivalently, the additional pressure equals the critical pressure after subtraction of systolic blood pressure (16 kPa). The case considered in the main text is shown in *red*

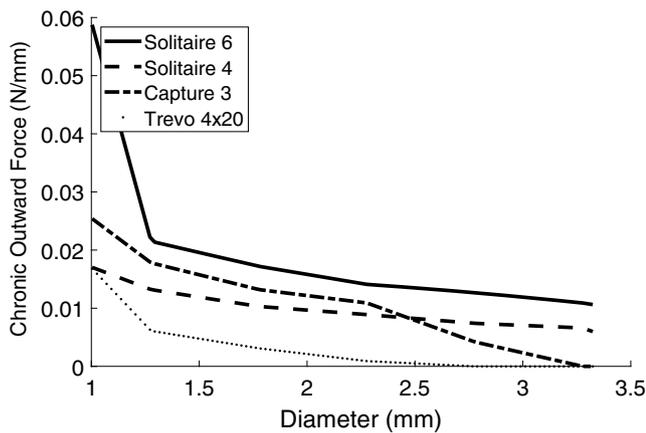

**Fig. C.1** Chronic outward force vs. diameter relationships for four commonly available stents: Solitaire 6 mm, Solitaire 4 mm, Capture 3 mm and Trevo 4 mm. Note the forces rapidly fall to zero as the stent expands

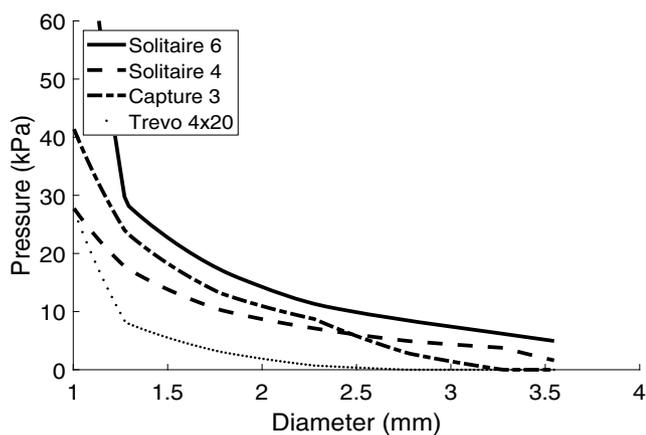

**Fig. C.2** Pressure-diameter curves for four commonly available stents: Solitaire 6 mm, Solitaire 4 mm, Capture 3 mm and Trevo 4 mm

equilibrium to obtain the relationship between  $f_a$  and  $f_p$  shown in Fig. B.2.

For each pair of values, we then computed the critical pressure, i.e. the pressure that should be applied to the arterial wall to cross the failure threshold of VSMCs (Fig. B.2, *above*). Subtracting systolic blood pressure (16 kPa) from the critical pressure, we obtained the additional pressure, namely the amount of pressure an interventional device should provide in order to treat vasospasm (Fig. B.2, *below*).

The results show that the minimum additional pressure a device should provide is about 5 kPa, while the maximum is about 11 kPa. Therefore, at most, the predictions for required stent pressure would increase to 11 kPa. Hence, the conclusion that pressures needed to treat vasospasm are attainable by stents and are an order of magnitude below the pressure used during balloon angioplasty treatment still holds.

### Appendix C

We start from a table of measurements of the chronic outward force (COF) exerted by the stents, expressed in N/mm; this represents the hoop force exerted by the stent divided by its length. Since the hoop force is measured in the circumferential direction, we use the identities in [20] to obtain:

$$P = \frac{COF}{lr},$$

where  $P$  is the pressure exerted by the stent,  $l$  the length of the stent and  $r$  the radius. We illustrate the COF-diameter relationship for the considered stents in Fig. C.1 and the corresponding pressure-diameter curves in Fig. C.2.

## References

- Honma Y, Fujiwara T, Irie K, Ohkawa M, Nagao S. Morphological changes in human cerebral arteries after percutaneous transluminal angioplasty for vasospasm caused by subarachnoid hemorrhage. *Neurosurgery*. 1995;36:1073–80. discussion 1080–1.
- Yamamoto Y, Smith RR, Berman DH. Mechanism of action of balloon angioplasty in cerebral vasospasm. *Neurosurgery*. 1992;30:1–5. discussion 5–6.
- Kobayashi H, Ide H, Aradachi H, Arai Y, Handa Y, Kubota T. Histological studies of intracranial vessels in primates following transluminal angioplasty for vasospasm. *J Neurosurg*. 1993;78:481–6.
- Macdonald RL, Wallace MC, Montanera WJ, Glen JA. Pathological effects of angioplasty on vasospastic carotid arteries in a rabbit model. *J Neurosurg*. 1995;83:111–7.
- Chan PD, Findlay JM, Vollrath B, Cook DA, Grace M, Chen MH, Ashforth RA. Pharmacological and morphological effects of in vitro transluminal balloon angioplasty on normal and vasospastic canine basilar arteries. *J Neurosurg*. 1995;83:522–30.
- Macdonald RL, Zhang J, Han H. Angioplasty reduces pharmacologically mediated vasoconstriction in rabbit carotid arteries with and without vasospasm. *Stroke*. 1995;26:1053–9. discussion 1059–60.
- Bhogal P, Loh Y, Brouwer P, Andersson T, Söderman M. Treatment of cerebral vasospasm with self-expandable retrievable stents: proof of concept. *J Neurointerv Surg*. 2017;9:52–9.
- Bhogal P, Paraskevopoulos D, Makalanda HL. The use of a stent-retriever to cause mechanical dilatation of a vasospasm secondary to iatrogenic subarachnoid haemorrhage. *Interv Neuroradiol*. 2017;23:330–5.
- Watton PN, Hill NA, Heil M. A mathematical model for the growth of the abdominal aortic aneurysm. *Biomech Model Mechanobiol*. 2004;3:98–113.
- Watton PN, Ventikos Y, Holzapfel GA. Modelling the growth and stabilization of cerebral aneurysms. *Math Med Biol*. 2009;26:133–64.
- Watton PN, Ventikos Y, Holzapfel GA. Modelling the mechanical response of elastin for arterial tissue. *J Biomech*. 2009;42:1320–5.
- Aparício P, Thompson MS, Watton PN. A novel chemo-mechanobiological model of arterial tissue growth and remodelling. *J Biomech*. 2016;49:2321–30.
- Hill MR, Duan X, Gibson GA, Watkins S, Robertson AM. A theoretical and non-destructive experimental approach for direct inclusion of measured collagen orientation and recruitment into mechanical models of the artery wall. *J Biomech*. 2012;45:762–71.
- Bevan T, Merabet N, Hornsby J, Watton PN, Thompson MS. A biomechanical model for fibril recruitment: Evaluation in tendons and arteries. *J Biomech*. 2018;74:192–6.
- Alford PW, Humphrey JD, Taber LA. Growth and remodeling in a thick-walled artery model: effects of spatial variations in wall constituents. *Biomech Model Mechanobiol*. 2008;7:245–62.
- Schrauwen JTC, Vilanova A, Rezakhanli R, Stergiopoulos N, van de Vosse FN, Bovendeerd PHM. A method for the quantification of the pressure dependent 3D collagen configuration in the arterial adventitia. *J Struct Biol*. 2012;180:335–42.
- Hong Z, Reeves KJ, Sun Z, Li Z, Brown NJ, Meininger GA. Vascular smooth muscle cell stiffness and adhesion to collagen I modified by vasoactive agonists. *PLoS One*. 2015;10:e0119533. <https://doi.org/10.1371/journal.pone.0119533>.
- Sehgel NL, Vatner SF, Meininger GA. “Smooth muscle cell stiffness syndrome”—revisiting the structural basis of arterial stiffness. *Front Physiol*. 2015;6:335.
- Yamaguchi-Okada M, Nishizawa S, Koide M, Nonaka Y. Biomechanical and phenotypic changes in the vasospastic canine basilar artery after subarachnoid hemorrhage. *J Appl Physiol*. 1985;99:2045–52.
- Fischell TA, Grant G, Johnson DE. Determinants of smooth muscle injury during balloon angioplasty. *Circulation*. 1990;82:2170–84.
- Cabrera MS, Oomens CWJ, Baaijens FPT. Understanding the requirements of self-expandable stents for heart valve replacement: radial force, hoop force and equilibrium. *J Mech Behav Biomed Mater*. 2017;68:252–64.
- Castaneda-Zuniga WR, Laerum F, Rysavy J, Rusnak B, Amplatz K. Paralysis of arteries by intraluminal balloon dilatation. *Radiology*. 1982;144:75–6.
- Herlihy JT, Murphy RA. Length-tension relationship of smooth muscle of the hog carotid artery. *Circ Res*. 1973;33:275–83.
- Wolf GL, Lentini EA. The influence of short-duration stretch on vasoconstrictor response in rabbit aortas. *Invest Radiol*. 1984;19:269–72.
- Wolf G, Lentini E, LeVeen R. Reduced vasoconstrictor response after angioplasty in normal rabbit aortas. *Am J Roentgenol*. 1984;142:1023–5.
- Faxon DP, Weber VJ, Haudenschild C, Gottsman SB, McGovern WA, Ryan TJ. Acute effects of transluminal angioplasty in three experimental models of atherosclerosis. *Arteriosclerosis*. 1982;2:125–33.
- Sanborn TA, Faxon DP, Haudenschild C, Gottsman SB, Ryan TJ. The mechanism of transluminal angioplasty: evidence for formation of aneurysms in experimental atherosclerosis. *Circulation*. 1983;68:1136–40.
- Consigny PM, Tulenko TN, Nicosia RF. Immediate and long-term effects of angioplasty-balloon dilation on normal rabbit iliac artery. *Arteriosclerosis*. 1986;6:265–76.
- Kwon HJ, Lim JW, Koh HS, Park B, Choi SW, Kim SH, Youm JY, Song SH. Stent-retriever angioplasty for recurrent post-subarachnoid hemorrhagic vasospasm—a single center experience with long-term follow-up. *Clin Neuroradiol*. 2018 Aug 6. [Epub ahead of print]
- Grytsan A, Eriksson TSE, Watton PN, Gasser TC. Growth description for vessel wall adaptation: a thick-walled mixture model of abdominal aortic aneurysm evolution. *Materials (Basel)*. 2017;10. <https://doi.org/10.3390/ma10090994>.
- Holzapfel GA, Gasser TC, Ogden RW. A New Constitutive Framework for Arterial Wall Mechanics and a Comparative Study of Material Models. *J Elast Phys Sci Solids*. 2000;61:1–48.
- Humphrey JD1, Baek S, Niklason LE. Biochemomechanics of cerebral vasospasm and its resolution: I. A new hypothesis and theoretical framework. *Ann Biomed Eng*. 2007;35:1485–97. <https://doi.org/10.1007/s10439-007-9321-y>.
- Baek S, Valentín A, Humphrey JD. Biochemomechanics of cerebral vasospasm and its resolution: II. Constitutive relations and model simulations. *Ann Biomed Eng*. 2007;35:1498–509. <https://doi.org/10.1007/s10439-007-9322-x>.
- Watton P, Ventikos Y. Modelling evolution of saccular cerebral aneurysms. *J Strain Analysis*. 2009;44:375–89. <https://doi.org/10.1243/03093247JSA492>.
- Watton PN, Hill NA. Evolving mechanical properties of a model of abdominal aortic aneurysm. *Biomech Model Mechanobiol*. 2009;8:25–42. <https://doi.org/10.1007/s10237-007-0115-9>.