



Operative and radiographic acetabular component orientation in total hip replacement: Influence of pelvic orientation and surgical positioning technique



Megan Rutherford^a, John D. O'Connor^a, Harinderjit S. Gill^b, Janet Hill^c, David Beverland^c, Alex B. Lennon^a, Nicholas J. Dunne^{d,e,f,g,h,*}

^a School of Mechanical and Aerospace Engineering, Queen's University of Belfast, Belfast, UK

^b Department of Mechanical Engineering, University of Bath, Bath, UK

^c Primary Joint Unit, Musgrave Park Hospital, Belfast, UK

^d School of Mechanical and Manufacturing Engineering, Dublin City University, Stokes Building, Collins Avenue, Dublin 9, Ireland

^e Centre for Medical Engineering Research, School of Mechanical and Manufacturing Engineering, Dublin City University, Stokes Building, Collins Avenue, Dublin 9, Ireland

^f School of Pharmacy, Queen's University Belfast, 97 Lisburn Road, Belfast BT9 7BL, UK

^g Trinity Centre for Bioengineering, Trinity Biomedical Sciences Institute, Trinity College Dublin, Dublin 2, Ireland

^h Department of Mechanical and Manufacturing Engineering, School of Engineering, Trinity College Dublin, Dublin 2, Ireland

ARTICLE INFO

Article history:

Received 26 June 2018

Revised 12 November 2018

Accepted 4 December 2018

Keywords:

Pelvic orientation

Mechanical alignment guide

Transverse acetabular ligament

Acetabular component inclination

ABSTRACT

Orthopaedic surgeons often experience a mismatch between perceived intra-operative and radiographic acetabular cup orientation. This research aimed to assess the impact of pelvic orientation and surgical positioning technique on operative and radiographic cup orientation.

Radiographic orientations for two surgical approaches were computationally simulated: a mechanical alignment guide and a transverse acetabular ligament approach, both in combination with different pelvic orientations. Positional errors were defined as the difference between the target radiographic orientation and that achieved.

The transverse acetabular ligament method demonstrated smaller positional errors for radiographic version; $4.0^\circ \pm 2.9^\circ$ as compared to $9.4^\circ \pm 7.3^\circ$ for the mechanical alignment guide method. However, both methods resulted in similar errors in radiographic inclination. Multiple regression analysis showed that intraoperative pelvic rotation about the anterior-posterior axis was a strong predictor for these errors ($B_{TAL} = -0.893$, $B_{MAG} = -0.951$, $p < 0.01$).

Application of the transverse acetabular ligament method can reduce errors in radiographic version. However, if the orthopaedic surgeon is referencing off the theatre floor to control inclination when operating in *lateral decubitus*, this is only reliable if the pelvic sagittal plane is horizontal. There is currently no readily available method for ensuring that this is the case during total hip replacement surgery.

© 2019 IPPEM. Published by Elsevier Ltd. All rights reserved.

1. Introduction

Current survivorship of a primary total hip replacement (THR) exceeds 90% at ten years [1]. Despite this success, negative outcomes such as dislocation [2] and wear [3] persist. Mal-alignment of the implanted acetabular component is one factor that has been implicated [3–5]. Great variability in acetabular component orientation is currently observed from post-operative radiographs [6–8].

A number of factors contribute to this variation with the most important being intra-operative pelvic orientation [9–10].

During THR, the acetabular component is inserted into the acetabulum using an introducer. The acetabular component axis is usually co-linear with the handle of the introducer and perpendicular to the face of the acetabular component being inserted. Acetabular component orientation is currently defined in relation to this axis in terms of inclination and version for both the operative and radiographic reference frames [11].

When using a mechanical alignment guide (MAG) in *lateral decubitus*, the operative inclination is referenced off the theatre floor (as a surrogate for the pelvic sagittal plane) and operative version is referenced from the surgical theatre table longitudinal axis (as a

* Corresponding author at: Centre for Medical Engineering Research, School of Mechanical and Manufacturing Engineering, Dublin City University, Stokes Building, Collins Avenue, Dublin 9, Ireland.

E-mail address: nicholas.dunne@dcu.ie (N.J. Dunne).

surrogate for the anterior pelvic plane, APP). In reality, the APP is rarely parallel to the patient's coronal plane, and the pelvic sagittal plane may not be parallel to the theatre floor as a result of pre-operative patient positioning and intra-operative pelvic movement [9]. Angles referenced from external theatre landmarks will, therefore, become *apparent* angles for operative inclination and version. Discrepancies between *true* (relative to pelvic sagittal plane and APP) and *apparent* (relative to theatre floor and table) operative acetabular component orientation will contribute to inconsistencies between the orthopaedic surgeon's expectations and the reality of post-operative X-ray measurements when using a MAG approach.

The transverse acetabular ligament (TAL) has been used to determine a patient-specific operative version relative to the APP [12]. TAL is independent of patient position but does not provide a solution for operative inclination. To control operative inclination, TAL is often used with a MAG or freehand approach. Pelvic mal-positioning and patient-specific TAL version will contribute to radiographic variability when using this approach.

Post-operatively and intra-operatively there is significant variation in the orientation of the APP with respect to the coronal plane of the patient [13]. This variation is commonly referred to as anterior and posterior pelvic tilt. This tilt, or movement, occurs as a result of flexion or extension of the lumbar spine which results in posterior and anterior tilt of the pelvis respectively. Because the X-ray is taken normal to the patient's coronal plane, pelvic tilt impacts the angle of radiographic version and, to a lesser degree, inclination [14]. Previous work [15–19] has analysed the discrepancy between the 3D orientation (operative or CT) and radiographic orientation of the acetabular component relative to the pelvis. However, the influence of surgical approach has not been explicitly analysed in relation to operative and radiographic acetabular cup orientation.

The aim of this research was to assess the impact of surgical positioning technique on operative and radiographic cup orientation for different pelvic orientations. Two different surgical techniques were simulated using the theory of rigid body transformations. The first used the surgical theatre table longitudinal axis to control operative version. This is equivalent to using the “version guide” on a MAG. The second simulated surgical technique used the TAL. For operative inclination, both techniques used the theatre floor. These approaches are the most commonly adopted within the UK with more than 50% of orthopaedic surgeons using them during THR [20]. Our hypothesis was that the TAL method would result in better control over acetabular component positioning relative to the pelvis when compared to the MAG method.

2. Method

2.1. Defining acetabular orientation

Acetabular orientation has previously been defined by inclination and version for both the operative and radiographic reference frames [11]. However, these definitions fail to take into account pelvic orientation [11]. To account for the impact of pelvic orientation, this paper proposes new definitions (Figs. 1–3).

Apparent operative acetabular cup orientation is the orientation of the acetabular component axis relative to external landmarks such as the surgical theatre floor and wall, intra-operatively, as perceived by orthopaedic surgeons. *Apparent operative inclination* (AOI) was defined as the angle between the acetabular component axis and the surgical theatre floor (Fig. 1). *Apparent operative version* (AOV) was defined as the angle between the acetabular component axis and the surgical theatre table longitudinal axis as projected onto the surgical theatre floor (Fig. 2).

True operative acetabular orientation represents the orientation of the acetabular component axis relative to internal pelvic land-

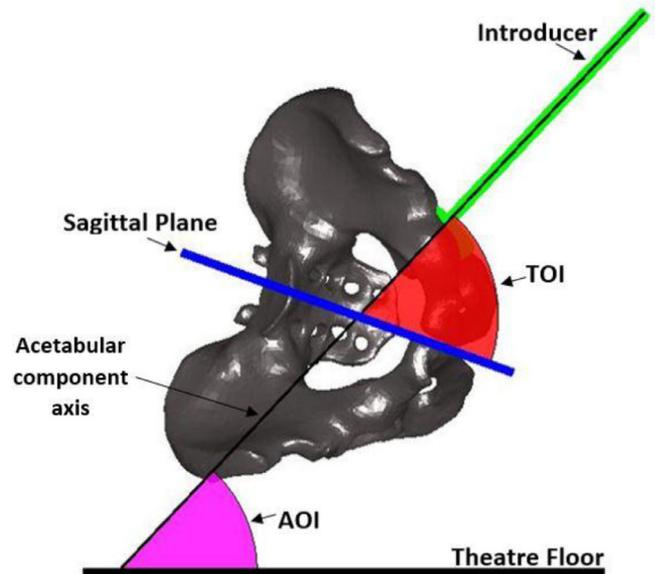


Fig. 1. Apparent (AOI) and True Operative Acetabular Inclination (TOI). TOI is the angle between the acetabular component axis and the pelvic sagittal plane. AOI is the angle between the acetabular component axis and the surgical theatre floor.

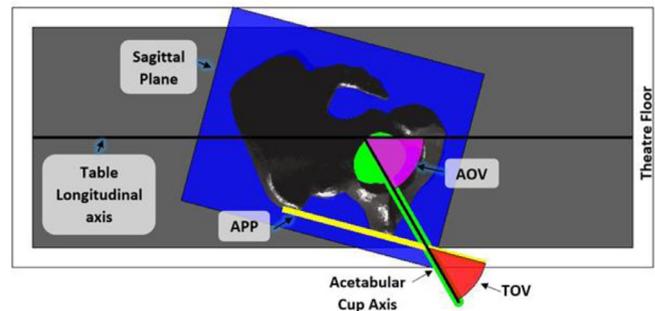


Fig. 2. Apparent (AOV) and True Operative Acetabular Version (TOV). AOV is the angle between acetabular component axis and surgical theatre table longitudinal axis as projected onto the surgical theatre floor. TOV is the angle between the acetabular component axis and anterior pelvic plane (APP) as projected onto the pelvic sagittal plane.

marks such as the APP intra-operatively. *True operative inclination* (TOI) was defined as the angle between the acetabular component axis and the pelvic sagittal plane (Fig. 1). *True operative version* (TOV) was the angle between the acetabular component axis and the APP as projected onto the pelvic sagittal plane (Fig. 2).

Radiographic inclination and version are the measurements routinely referenced in practice that do not take into account anterior and posterior pelvic tilt. *Radiographic inclination* (RI) was calculated as the angle between the pelvic longitudinal axis and the acetabular component axis projected onto the coronal plane (Fig. 3) [11]. *Radiographic version* (RV) was determined from the relative sizes of the minor and major diameters [21] of the projected acetabular component face (Fig. 3). *Neutralised radiographic acetabular component orientation* was defined as the radiographic inclination (NRI) and version (NRV) that would result from an X-ray for which the pelvis was neutral. Radiographic pelvic neutrality was achieved when the APP was parallel to the coronal plane (Fig. 3).

2.2. Intra-operative pelvic orientation

A Sawbones™ pelvis (Sawbones Europe AB, Sweden) was surface-scanned using a coordinate measurement machine

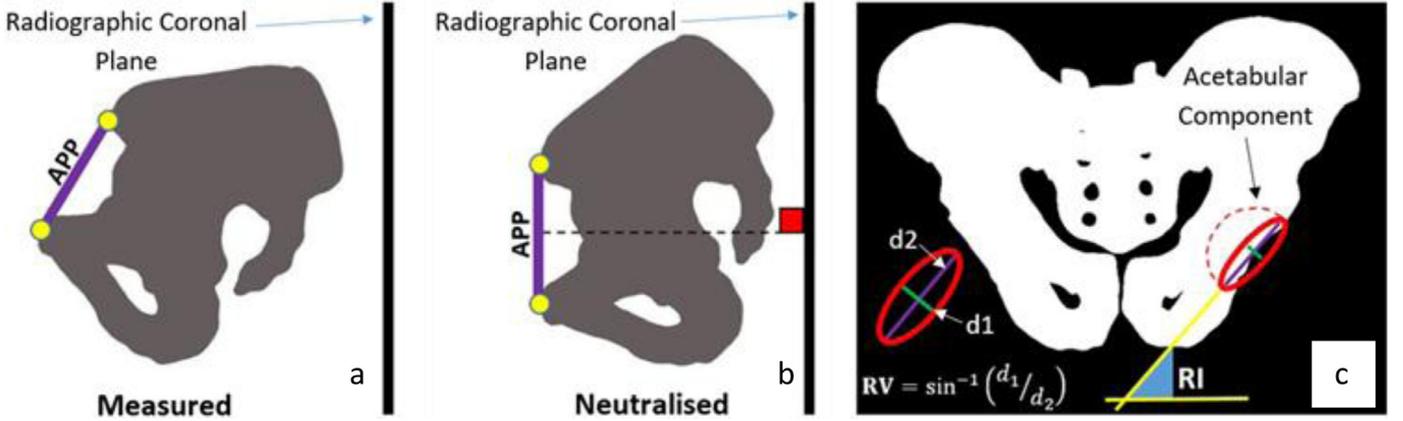


Fig. 3. Measured and Neutralised Radiographic Measurements: (a and c) radiographic inclination (RI) and Version (RV) are measures of inclination and version taken from an anterior-posterior radiograph for which the orientation of the pelvis has not been accounted for; (b and c) neutralised radiographic inclination (NRI) and version (NRV) are measures of radiographic inclination and version taken from an anterior-posterior radiograph for which the orientation of the pelvis has been accounted for.

(Hexagon Global Status CMM 092008, Hexagon Manufacturing Intelligence, UK) equipped with a Renishaw PH10M probe head (Renishaw plc, UK) and Nikon LC50 Laser with Nikon Focus scan software (Nikon Corp., Japan) to produce a high density point cloud, which was converted into a surface mesh using 3D scanning and computer aided design (CAD) software (Rapidform XOR, 3D Systems Inc., USA and PTC Creo, PTC Inc., USA) and imported into MATLAB (2015b, The MathWorks Inc., USA). The pelvic model was initially orientated to match the idealised *neutral* pelvic orientation for a patient undergoing THR of a left hip in *lateral decubitus*. Operative pelvic neutrality was achieved when the pelvic APP was parallel to the surgical theatre longitudinal axis, and the pelvic sagittal plane was parallel to the surgical theatre floor.

Coordinates for the hip joint centre of rotation (\hat{C}_N ; COR) relative to a neutral pelvis in the operative reference frame were acquired (Fig. 4). Rotation of the neutral pelvis about its three axes (Fig. 4) was achieved using Eq. 1. Regardless of approach, the rotated position of the hip COR (\hat{C}_R) represents the pivot about which the orthopaedic surgeon orientates the acetabular component. Rotation of the upper (left) hemi-pelvis about its longitudinal axis, $R_x(\theta_{rot})$, intra-operatively was regarded as internal (+) / external (-) rotation. Rotation of the upper (left) hemi pelvis about its anterior-posterior axis, $R_y(\theta_{add})$, was regarded as abduction (+) / adduction (-). Rotation of the pelvis about its transverse axis, $R_z(\theta_{tilt})$, intra-operatively was termed anterior (+) / and posterior (-) pelvic tilt.

$$\hat{C}_R = R_x(\theta_{rot})R_z(\theta_{add})R_y(\theta_{tilt})\hat{C}_N \quad (1)$$

2.3. Mechanical alignment guide approach

With the pelvis mal-rotated, the acetabular component axis was angled at 45° relative to the theatre floor (AOI) and 20° relative to the long axis of the surgical theatre table as projected onto the surgical theatre floor (AOV) [10,21–22]. This was achieved by rotating the acetabular component relative to the axes of its local coordinate frame (\hat{e}_1 , \hat{e}_2 and \hat{e}_3 , Fig. 4). The surgical error (i.e., the orthopaedic surgeon's ability to achieve their target orientation) when using the MAG approach was also incorporated. The surgical errors for version (SE_{MAGV} , $3 \pm 5^\circ$) and inclination (SE_{MAGI} , $-3 \pm 5^\circ$) were based on an assumed normal distribution defined by mean and standard deviation error values from an experimental study of surgical accuracy [23]. The resultant position of the acetabular cup axis for the MAG approach (\hat{I}_M) was obtained using Eq. 2, which orientated the introducer such that it matched

Murray's definitions for operative acetabular orientation.

$$\hat{I}_M = (R_y(-AOV + SE_{MAGV})R_z(AOI + SE_{MAGI})\hat{e}_1) + \hat{C}_R \quad (2)$$

2.4. Transverse acetabular ligament approach

For the TAL approach, a TAL axis was introduced relative to the neutral pelvis (\hat{I}_N ; Fig. 5). This axis was assigned a case-specific TAL version (TOV) and surgical error (SE_{TALV} , Eq. (3)). The location of the TAL axis relative to the mal-rotated intra-operative pelvis (\hat{I}_R) was obtained using Eq. (4).

$$\hat{I}_N = (R_y(-TOV + SE_{TALV})\hat{e}_3) + \hat{C}_N \quad (3)$$

$$\hat{I}_R = R_x(\theta_{rot})R_z(\theta_{add})R_y(\theta_{tilt})\hat{I}_N \quad (4)$$

With the pelvis and consequently the TAL axis mal-rotated, the acetabular component axis was angled at 45° relative to the surgical theatre floor (AOI) about the TAL axis. A custom solver, Eq. (5), was developed to determine the angle (α) that the acetabular cup axis for the TAL method (\hat{I}_T) would have to rotate about the \hat{I}_R axis to provide an AOI of 45°, between the introducer and theatre floor (\hat{I}_{Txz} ; Fig. 5). Surgical errors for the TAL method (SE_{TALI} , $-3 \pm 5^\circ$, and SE_{TALV} , $0 \pm 7^\circ$) were based on the findings of Grammatopoulos et al. [23]. This in turn provided the resultant intra-operative location of the acetabular cup axis when using the TAL approach (\hat{I}_T).

$$f(\alpha) = (AOI + SE_{TALI}) - \cos^{-1}(\hat{I}_T \cdot \hat{I}_{Txz}) \quad (5)$$

2.5. Analysis

Measures for apparent operative, true operative, radiographic, and neutralised radiographic acetabular orientation were obtained from the model. Variation in TAL version [24], surgical error [23] and pelvic orientation [9] were incorporated into the models to induce variation in the aforementioned measures. For each factor, normal distributions were fitted to clinical data from the literature and sampled randomly ($n=1000$). Since one of the main consequences of sub-optimal acetabular cup positioning (dislocation) is relatively rare, a large sample size was required in order to include extreme cases. Radiographic projection was modelled according to Freud et al. [25] with a source-to-image distance of 1 m. For repeatability, the source was aligned with the pubic symphysis of the pelvic model whilst the rearmost portion of the pelvic model was aligned with the image plane. As the rearmost portion of the pelvis is aligned with the image plane (supported by the table in practice), if the pelvic tilt changes, the distance between

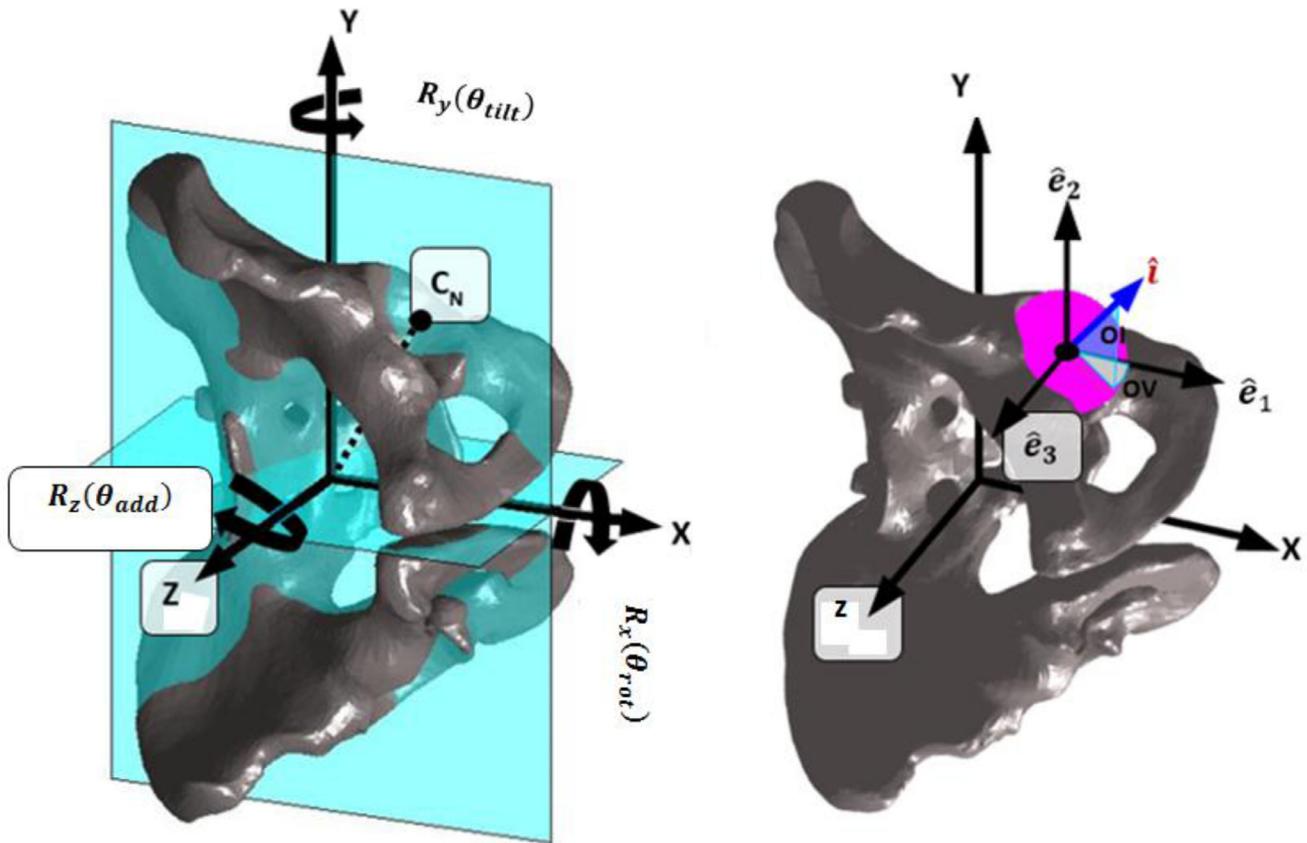


Fig. 4. Schematic diagram highlighting the pelvic (X,Y,Z) and acetabular cup (\hat{e}_1 , \hat{e}_2 , \hat{e}_3) coordinate frames, the hip joint centre of rotation (\hat{C}_N), and acetabular cup axis (\hat{i}).

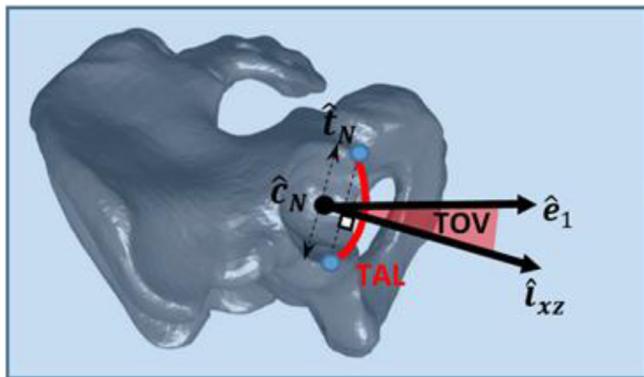


Fig. 5. Schematic diagram depicting a neutral transverse acetabular ligament (TAL) axis (\hat{i}_N) at a case-specific TOV.

the pubic symphysis and the source would change (as would occur in surgical practice). Therefore there is not a single fixed distance between the pelvis and the source. Target radiographic orientation was the neutralised radiographic orientation that would have been achieved if the acetabular component had been implanted into a neutral pelvis intra-operatively in the absence of surgeon error. A case was classified as on-target if its neutralised radiographic orientation was within 10° of the target radiographic orientation, based on ranges presented by Lewinnek et al. [21]. For each case, a positional error was calculated. This was defined as the difference between the neutralised radiographic orientation achieved and the target radiographic orientation. Multiple linear regression, general mixed models, and Chi Square analyses were conducted

using SPSS (v22, IBM, USA). Multiple linear regression was used to determine the relationship between positional errors and surgical factors. General mixed models with Bonferroni post-hoc analysis were used to test for statistical differences between measures of orientation. Chi Square analysis was conducted to determine if there was a significant interaction between safe placement and the choice of guidance technique. Further analysis was conducted using the Statistics Toolbox and plotting capabilities within MATLAB® (2015b, The Mathworks Inc., USA). A p -value of 0.05 was considered significant.

3. Results

3.1. Inclination

No statistical difference ($p=0.243$) was observed between the TAL and MAG methods across the measures of inclination (Fig. 6). However, each of the four measures for inclination were mutually statistically different from each other ($p < 0.001$). Despite statistical significance, there was negligible difference between the mean AOI and TOI (MAG = 0.5° , TAL = 0.8° ; Table 1). The same was true of the difference between the mean RI and NRI (MAG = 1.1° , TAL = 1.1°).

Regardless of the small deviation in the mean angle of inclination across all measures, there was an initial increase in the ranges between AOI ($\Delta AOI_{MAG} = 20.4^\circ$, $\Delta AOI_{TAL} = 20.4^\circ$) and TOI groups ($\Delta TOI_{MAG} = 40.9^\circ$, $\Delta TOI_{TAL} = 45.2^\circ$). Despite an orthopaedic surgeon's level of control over the orientation of the introducer relative to the surgical theatre floor, these results indicate that intra-operative pelvic orientation can double the range in inclination that an orthopaedic surgeon would expect to see post-operatively.

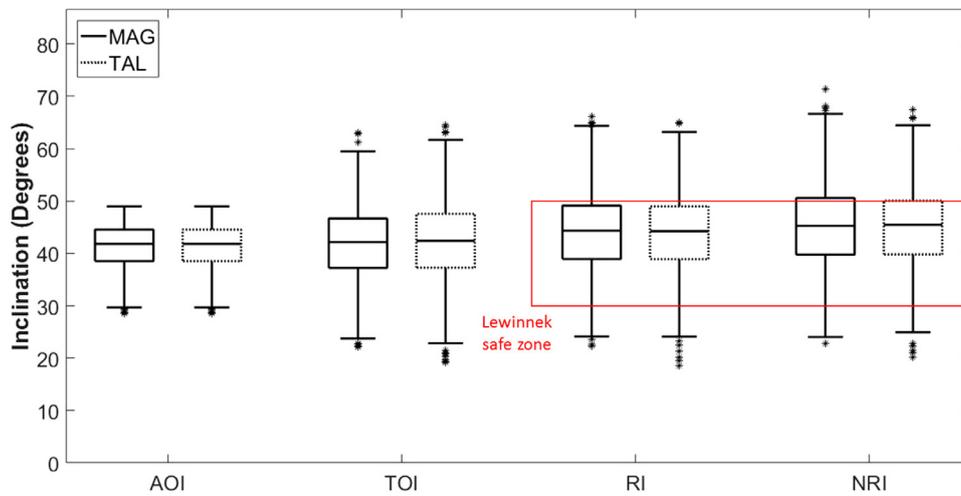


Fig. 6. Measures of Inclination. No statistical differences were observed between approaches ($p=0.243$). Both methods exhibit similar control over TOI. Operative pelvic orientation doubles the range in inclination that an orthopaedic surgeon would expect to see post-operatively. Outliers (denoted by *) are defined as those points above $Q3 + 1.5(Q3 - Q1)$ or below $Q1 - 1.5(Q3 - Q1)$, where $Q1$ and $Q3$ are the first and third quartiles, respectively.

Table 1
Minimum, maximum, mean, and standard deviation for inclination and version measures for the MAG and TAL method.

	Mechanical Alignment Guide (MAG)				Transverse Acetabular Ligament (TAL)			
	Min (degrees)	Max (degrees)	Mean (degrees)	SD (degrees)	Min (degrees)	Max (degrees)	Mean (degrees)	SD (degrees)
AOI	28.6	49	41.4	4.2	28.6	49	41.4	4.2
TOI	22.1	63.1	41.9	7.1	19.2	64.5	42.2	7.8
RI	22.3	66.2	44.2	7.6	18.5	65.1	43.9	7.6
NRI	22.7	71.4	45.3	7.9	20.2	67.4	45	7.5
PI ^a	0	25	6.6	5	0	27.6	6.4	5
AOV	2.2	23.9	16.1	4.4	-34.8	71.9	17.7	19
TOV	-40.6	62.6	16.5	16.8	-8.7	41.3	17.9	9.3
RV	-35.5	37.4	3.8	12.6	-24.4	30.1	5.1	8.5
NRV	-32.1	44	8.8	11.8	-9.1	35.2	10.1	7
PV ^b	0	42.7	9.4	7.3	0	17.4	4	2.9

^a PI: Absolute positional error in inclination.
^b PV: Absolute positional error in version.

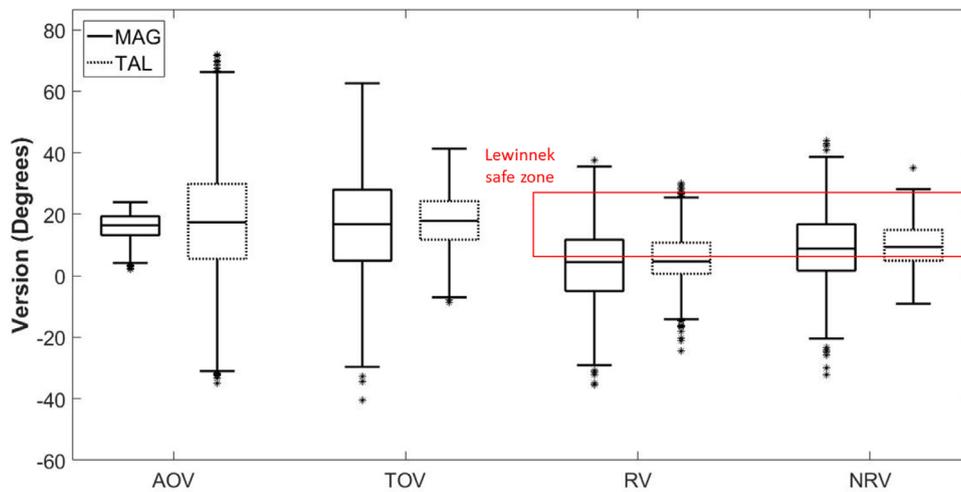


Fig. 7. Measures of version. Statistical differences were observed between approaches ($p < 0.01$). TAL method results in better control of TOV when compared to MAG. Outliers (denoted by *) are defined as those points above $Q3 + 1.5(Q3 - Q1)$ or below $Q1 - 1.5(Q3 - Q1)$, where $Q1$ and $Q3$ are the first and third quartiles, respectively.

3.2. Version

Unlike inclination, a statistical difference ($p < 0.001$) was observed between the TAL and MAG methods across measures of version (Fig. 7). For AOV, the MAG method exhibited tighter control ($\Delta AOV_{MAG} = 21.7^\circ$) when compared to the TAL method ($\Delta AOV_{TAL} = 106.7^\circ$). Despite this apparent increase in control, the

TAL method ($\Delta TOV_{TAL} = 50.1^\circ$) results in a smaller range of TOV when compared to the MAG method ($\Delta TOV_{MAG} = 103.2^\circ$). Linear regression showed the variability in TOV is predominantly accounted for by the variation in the natural target TAL version ($r = 0.75, p < 0.01$). From the orthopaedic surgeon's perspective, the angular orientation of the acetabular component may appear excessive when using the TAL method. However, as indicated by the

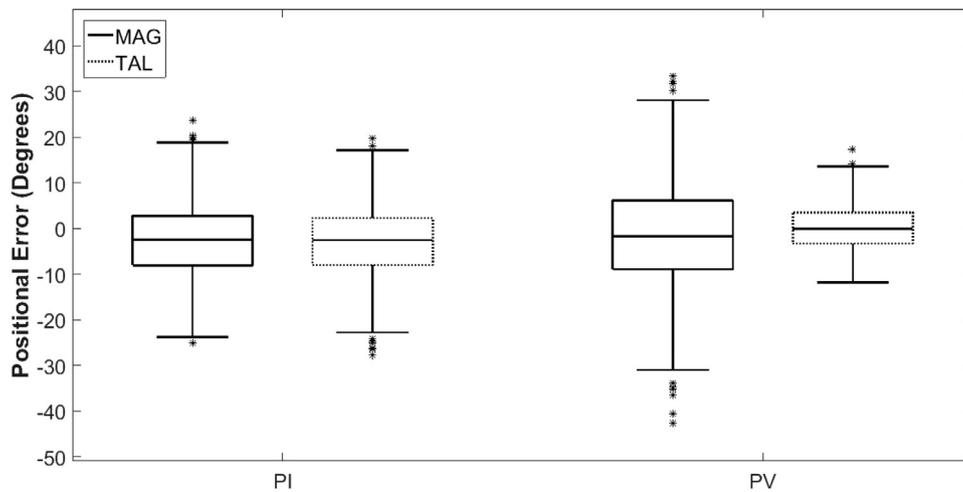


Fig. 8. TAL reduces positional errors for version (PV) but not for inclination (PI). Outliers (denoted by *) are defined as those points above $Q3 + 1.5(Q3 - Q1)$ or below $Q1 - 1.5(Q3 - Q1)$, where $Q1$ and $Q3$ are the first and third quartiles, respectively.

reduction in TOV over AOV, the TAL method results in better control over operative version.

AOV and TOV were considered statistically similar ($p=0.243$), while the other measures were all mutually statistically different ($p<0.001$). The introduction of anterior and posterior pelvic tilt alters the angle of version projected onto the coronal plane, accounting for differences between the operative measures of version and the radiographic version. Deviations between the mean TOV (MAG = 16.5° , TAL = 17.9°) and the mean NRV (MAG = 8.82° , TAL = 10.1°) reflect the inadequacy of the ellipse fitting method used to compute the three-dimensional version of the acetabular component from a two-dimensional radiograph.

3.3. Positional errors

Target radiographic inclination and version for the MAG method was 47.8° and 10.6° respectively when aiming for 45° of operative inclination and 20° of operative version. Due to the natural variation in TAL-based version, target radiographic inclination and version were case-specific for the TAL method even though target operative inclination was constant. Mean target radiographic inclination for the TAL method was 47.8° ($\pm 1.52^\circ$, min = 45.1° , max = 52.2°). Mean target radiographic version for the TAL method was 9.96° ($\pm 4.46^\circ$, min = 0.02° , max = 20.1°). Target radiographic inclination ($n=104/1,000$) and radiographic version ($n=148/1000$) for a number of TAL cases fell outside of the Lewinnek target zone²⁰ (Figs. 6 and 7). Thus, acetabular components may be classified as unsafe when using the Lewinnek target zone, despite being placed inside the allowable margin of error ($\pm 10^\circ$) relative to their intended orientation.

A Chi-square test of independence was calculated comparing the frequency of acetabular components placed safely when using the TAL and MAG method. A significant interaction was found (χ^2 (1, $n=1000$) = 150.3, $p<0.01$) between insertion methods and safe placement. With respect to placement within the safe zones for both radiological inclination and version, the TAL method ($n=778/1000$) exhibited a 33.7% increase in safe placement over the MAG method ($n=516/1000$).

For inclination error (Fig. 8, Table 2), multivariate linear regression showed that the strongest standardised coefficients (B), or predictors, were the orthopaedic surgeon's ability to achieve their desired target angle ($B_{MAG} = 1.02$, $B_{TAL} = 1.10$, $p<0.01$) and intra-operative control of pelvic adduction ($B_{MAG} = -0.95$, $B_{TAL} = -0.89$, $p<0.01$) for both MAG and TAL (Fig. 8, Table 2). For errors in version, the orthopaedic surgeon's ability to achieve their

desired target angle ($B_{MAG} = 0.711$, $p<0.01$) and intra-operative control of pelvic flexion were the strongest predictors ($B_{MAG} = 0.689$, $p<0.01$) for MAG. For TAL, only the orthopaedic surgeon's ability to achieve their desired target angle ($B_{TAL} = 0.708$, $p<0.01$) was a notable predictor of version error.

4. Discussion

We hypothesised that the TAL method would result in better control over acetabular component positioning relative to the pelvis when compared to the MAG method. The TAL method ($\Delta TOV = 50.0^\circ$) resulted in a smaller range of TOV when compared to the MAG method ($\Delta TOV = 103.2^\circ$). However, for TOI, the TAL method ($\Delta TOI = 45.3^\circ$) exhibited similar variability to the MAG method ($\Delta TOI = 41.0^\circ$). The TAL method uses a fixed internal patient-specific landmark for controlling operative version, which can counteract changes in pelvic tilt. However, as with the MAG method, it relies on the fixed external surgical theatre floor for controlling operative inclination. Overall, our hypothesis that the TAL method would lead to better control over acetabular component orientation was supported by the results herein.

For both methods, intra-operative pelvic orientation at least doubled the range in inclination that an orthopaedic surgeon would expect to see post-operatively. This is particularly influenced by pelvic adduction. However, high natural cup version combined with internal rotation can also be a contributing factor. Therefore, in *lateral decubitus*, the surgical theatre floor can only be used as a reliable landmark for operative inclination if the sagittal plane of the pelvis is horizontal.

Meermans et al. [26] conducted a clinical trial comparing the TAL and freehand techniques. From their findings, the TAL method was better at controlling radiological version than the MAG technique, which concurs with the findings from this study. The range in measured radiological version obtained using our theoretical model (MAG: -35.5° to 37.4° , TAL: -24.4° to 30.1°) differs from that obtained by Meermans et al. in a clinical setting (MAG: 2° – 35° , TAL: 2° – 25°). An advantage of the theoretical model is the spatial location of the acetabular component axis relative to the radiographic coronal plane is known. This enables differentiation between retroverted and anteverted acetabular components, which is not possible on the AP X-ray. Ignoring the possibility of retroversion by taking the absolute values of measured radiographic version only, the ranges obtained from the theoretical model (MAG: 0° – 37.4° , TAL: 0° – 30.1°) concurs with data reported by Meermans et al. [26].

Table 2

Prediction of inclination positional errors (PI) and version positional errors (PV) from intra-operative factors using multivariate regression standardised coefficients (B).

Predictor	Mechanical Alignment Guide (MAG)		Transverse Acetabular Ligament (TAL)	
	B	p	B	P
PI				
Constant (Intercept)	1	<0.001	0.832	<0.001
Operative Pelvic Rotation	0.24	<0.001	0.273	<0.001
Operative Pelvic Adduction	-0.951	<0.001	-0.893	<0.001
Operative Pelvic Flexion	0.198	<0.001	0.157	<0.001
Surgeon Inclination Error	1.024	<0.001	1.1013	<0.001
Model Fit	F(4, 995)=4,379, $p < 0.001$, $R^2 = 0.946$		F(4, 995)=2,451, $p < 0.001$, $R^2 = 0.908$	
PV				
Constant (Intercept)	0.925	<0.001	0.831	<0.001
Operative Pelvic Rotation	-0.626	<0.001	-0.09	<0.001
Operative Pelvic Adduction	-0.016	0.105	0.245	<0.001
Operative Pelvic Flexion	0.689	<0.001	-0.046	<0.001
Surgeon Version Error	0.711	<0.001	0.708	<0.001
Model Fit	F(4, 995)=10,678, $p < 0.001$, $R^2 = 0.977$		F(4, 995)=1,584, $p < 0.001$, $R^2 = 0.864$	

Meermans et al. [26] concluded that the TAL method was better at controlling radiological version based upon their radiographic outcomes being within the Lewinnek target zone [21]. Natural variation of TAL, [23] along with the natural variation in pelvic tilt, [13] may result in greater inter-patient variability with respect to measured radiological version. In this study, patient-specific targets for NRI and NRV were calculated. With respect to the Lewinnek target zone [21], 43% ($n = 430/1000$) of target neutralised radiographic orientations fell outside for TAL. Other studies have also noted potential problems with using global, rather than patient-specific, targets; e.g., Abdel et al. [6] illustrated that 58% of dislocations from their prospective study were located within the Lewinnek target (safe) zone. To date, no consensus regarding safe orientation of the acetabular component exists [2,8,27]. Irrespective of the safe zone used to assess radiographic success post-operatively, TAL has been associated with a reduced rate of dislocation [12].

A potential limitation of this study is the use of a single order of rotations. However, the same pelvic orientation can result from differently ordered rotations. Thus, changing the order of the rotations only varies the mapping procedure required to gain a particular pelvic orientation. If we were to include multiple mappings, duplicate pelvic positions would result, which may bias the data and subsequent observations from this study. A limitation of the theoretical model was that it was based on clinical data from a limited number of institutions [9,23,24]. For example, the extent of pelvic mal-positioning may be influenced by the type of intraoperative patient support. Additionally, in practice, an orthopaedic surgeon will be able to use their experience to avoid extreme orientations that are not accounted for in the model. This study was performed on a single, representative pelvic shape. Since the key variables are angles (as opposed to lengths), we expect that data and study observations will apply to a wide variation of pelvic shapes. However, this has not been analysed here and these methods could be applied in future studies.

Computer Aided Orthopaedic Surgery (CAOS) has been shown to reduce the variance in acetabular component placement [28] by determining the intra-operative pelvic orientation. This is most accurately achieved using an image-based system that recognises the internal anatomy during THR surgery and then builds a three-dimensional image of the pelvis from this. In contrast, image-free systems are more widely used to build a three-dimensional image by referencing bony landmarks on the pelvis through skin, which in turn introduces errors [29]. Within the United Kingdom, CAOS is used in less than 1% of THR surgeries [30]. This may be due to cost, increased operative time, and lack of published benefit [31,32]. For example, Lass et al. [33] illustrated no significant difference

between the MAG method and an image free system for controlling TOI.

5. Conclusion

In this study, which simulated two different surgical techniques, the TAL method exhibited greater control over radiographic version and placed 33.7% more acetabular components in the hypothetical target zone when compared to the application of the MAG method. However, with respect to inclination, both the TAL and MAG methods performed poorly when the sagittal pelvic plane was not parallel to the surgical theatre floor. Consequently, there is an imperative to find an affordable and practical method to ensure the sagittal plane of the pelvis is parallel to the surgical theatre floor at the time of acetabular component insertion.

Author's contribution statement

Megan Rutherford: Contributed to acquisition, analysis, interpretation of data and drafted the paper.

John D. O'Connor: Critical review and revision of the draft manuscript.

Harinderjit S. Gill: Critical review of the draft manuscript.

Janet Hill: Contributed to research design, critical review of the draft manuscript, and approval of the submitted manuscript.

David Beverland: Contributed to research design, critical review of the draft manuscript, and approval of the submitted manuscript.

Alex B. Lennon: Contributed to research design, critical review of the draft manuscript, and approval of the submitted manuscript.

Nicholas J. Dunne: Contributed to research design, critical review of the draft manuscript, and approval of the submitted manuscript.

Conflicts of interest

There are no conflicts of interest.

Funding

M. Rutherford would like to acknowledge the financial support of the Belfast Arthroplasty Research Trust for this study. D. E. Beverland has stated that he, along with the Belfast Health and Social Care Trust, has received funding from Depuy Synthes for this study.

Ethical approval

No ethical approval was required for this study.

References

- [1] Kim Y, Park J, Kim J, Kim I. Twenty five to twenty seven year results of a cemented vs a cementless stem in the same patients younger than 50 years of age. *J Arthroplasty* 2016;31(3):662–7.
- [2] Biedermann R, Tonin A, Krismer M, Rachbauer F, Eibl G, Stöckl B. Reducing the risk of dislocation after total hip arthroplasty: the effect of orientation of the acetabular component. *Bone Joint J* 2005;87-B(6):762–9.
- [3] Wan Z, Boutary M, Dorr LD. The influence of acetabular component position on wear in total hip arthroplasty. *J Arthroplasty* 2008;23(1):51–6.
- [4] Little N, Busch C, Gallagher J, Rorabeck CH, Bourne RB. Acetabular polyethylene wear and acetabular inclination and femoral offset. *Clin Orthop Relat Res* 2009;467(11):2895–900.
- [5] von Knoch M, Berry DJ, Harmsen WS, Morrey BF. Late dislocation after total hip arthroplasty. *J Bone Joint Surg Am* 2002;84-A(11):1949–53.
- [6] Abdel M, Roth P, Jennings M, Hanssen AD, Pagnano MW. What safe zone? The vast majority of dislocated THAs are within the Lewinnek safe zone for acetabular component position. *Clin Orthop Relat Res* 2015;474(2):386–91.
- [7] Langton DJ, Joyce TJ, Jameson SS, Lord J, Van Orsouw M, Holland JP, et al. Adverse reaction to metal debris following hip resurfacing. *J Bone Joint Surg Br* 2011;93-B(2):164–71.
- [8] Danoff JR, Bobman JT, Cunn G, Murtaugh T, Gorroochurn P, Geller JA, et al. Redefining the acetabular component safe zone for posterior approach total hip arthroplasty. *J Arthroplasty* 2016;31(2):506–11.
- [9] Grammatopoulos G, Pandit HG, da Assunção R, Taylor A, McLardy-Smith P, De Smet KA, et al. Pelvic position and movement during hip replacement. *Bone Joint J* 2014;96-B(7):876–83.
- [10] Beverland DE, O'Neill CK, Rutherford M, Molloy D, Hill JC. Placement of the acetabular component. *Bone Joint J* 2016;98-B(1 Suppl A):37–43.
- [11] Murray DW. The definition and measurement of acetabular orientation. *J Bone Joint Surg Br* 1993;75-B(2):228–32.
- [12] Archbold HA, Mockford B, Molloy D, McConway J, Ogonda L, Beverland D. The transverse acetabular ligament: an aid to orientation of the acetabular component during primary total hip replacement: A preliminary study of 1000 cases investigating postoperative stability. *J Bone Joint Surg Br* 2006;88-B(7):883–886.
- [13] Murphy WS, Klingenstein G, Murphy SB, Zheng G. Pelvic tilt is minimally changed by total hip arthroplasty. *Clin Orthop Relat Res* 2013;471(2):417.
- [14] Haenle M, Heitner A, Mittelmeier W. Assessment of cup position from plain radiographs: impact of pelvic tilting. *Surg Radiol Anat* 2007;29(1):29–35.
- [15] Grammatopoulos G, Pandit HG, da Assunção R, McLardy-Smith P, De Smet KA, Gill HS, et al. The relationship between operative and radiographic acetabular component orientation: which factors influence resultant cup orientation? *Bone Joint J* 2014;96-B(10):1290–7.
- [16] Davda K, Smyth N, Cobb JP, Hart AJ. 2D measurements of cup orientation are less reliable than 3D measurements: a retrospective study of 87 metal-on-metal hips. *Acta Orthop* 2015;86(4):485–90.
- [17] Wassilew GI, Heller MO, Diederichs G, Janz V, Wenzl M, Perka C. Standardized AP radiographs do not provide reliable diagnostic measures for the assessment of acetabular retroversion. *J Orthop Res* 2012;30(9):1369–76.
- [18] Schwarz TJ, Weber M, Dornia C, Worlicek M, Renkawitz T, Grifka J, et al. Correction of pelvic tilt and pelvic rotation in cup measurement after THA - an experimental study. *Rofo* 2017;189(9):864–73.
- [19] Derbyshire B. Correction of acetabular cup orientation measurements for X-ray beam offset. *Med Eng Phys* 2008;30(9):1119–26.
- [20] Rutherford M, O'Connor JD, Hill JC, Beverland DE, Lennon AB, Dunne NJ. Patient positioning and cup orientation during total hip arthroplasty: assessment of current UK practice. *Hip Int* 2018 [Epub ahead of print].
- [21] Lewinnek G, Lewis J, Tarr R, Compere CL, Zimmerman JR. Dislocations after total hip-replacement arthroplasties. *J Bone Joint Surg* 1978;60(2):217–20.
- [22] Barrack RL. Dislocation after total hip arthroplasty: implant design and orientation. *J Am Acad Orthop Surg* 2003;11(2):89–99.
- [23] Grammatopoulos G, Alvand A, Monk AP, Mellon S, Pandit H, Rees J, Gill HS, Murray DW. Surgeons' accuracy in achieving their desired acetabular component orientation. *Bone Joint J* 2016;98-A(17):72.
- [24] Merle C, Grammatopoulos G, Waldstein W, Pegg E, Pandit H, Aldinger PR, Gill HS, Murray DW. Comparison of native anatomy with recommended safe component orientation in total hip arthroplasty for primary osteoarthritis. *Bone Joint J* 2013;95-A(7):1721–7.
- [25] Freud N, Duvauchelle P, Létang JM, Babot D. Fast and robust ray casting algorithms for virtual X-ray imaging. *Nucl Instrum Methods Phys Res Sect B Beam Interact with Mater Atoms* 2006;248:175–80.
- [26] Meermans G, Van Doorn WJ, Koenraadt K, Kats J. The use of the transverse acetabular ligament for determining the orientation of the components in total hip replacement. *Bone Joint J* 2014;96-B(3):312–18.
- [27] Elkins J, Callaghan J, Brown T. The 'Landing zone' for wear and stability in total hip arthroplasty is smaller than we thought: a computational analysis. *Clin Orthop Relat Res* 2014;473(2):441–52.
- [28] Digioia AM III, Jaramaz B, Plakseychuk AY, Moody JE Jr, Nikou C, Labarca RS, et al. Comparison of a mechanical acetabular alignment guide with computer placement of the socket. *J Arthroplasty* 2002;17(3):359–64.
- [29] Lin F, Lim D, Wixson RL, Milos S, Hendrix RW, Makhosous M. Limitations of imageless computer-assisted navigation for total hip arthroplasty. *J Arthroplasty* 2011;26(4):596–605.
- [30] UK National Joint Registry 10th Annual Report, http://www.njrcentre.org.uk/njrcentre/Portals/0/Documents/England/Reports/10th_annual_report/NJR%2010th%20Annual%20Report%202013%20B.pdf ; 2013.
- [31] Najarian BC, Kilgore JE, Markel DC. Evaluation of component positioning in primary total hip arthroplasty using an imageless navigation device compared with traditional methods. *J Arthroplasty* 2009;24(1):15–21.
- [32] Sikorski JM, Chauhan S. Computer-assisted orthopaedic surgery: do we need CAOS? *J Bone Joint Surg Br* 2003;85-B(3):319–23.
- [33] Lass R, Kubista B, Olischar B, Frantal S, Windhager R, Giurea A. Total hip arthroplasty using imageless computer-assisted hip navigation: a prospective randomized study. *J Arthroplasty* 2014;29(4):786–91.