



2D monolithic silicon-diode array detectors in megavoltage photon beams: does the fabrication technology matter? A medical physicist's perspective

N. Stansook^{1,2} · G. Biasi¹ · K. Utitsarn^{1,5} · M. Petasecca^{1,3} · P. Metcalfe¹ · M. Carolan^{3,4} · M. L. F. Lerch^{1,3} · V. L. Perevertaylo⁶ · T. Kron^{1,7,8} · A. B. Rosenfeld^{1,3}

Received: 24 September 2018 / Accepted: 19 February 2019 / Published online: 21 February 2019
© Australasian College of Physical Scientists and Engineers in Medicine 2019

Abstract

A family of prototype 2D monolithic silicon-diode array detectors (MP512, Duo, Octa) has been proposed by the Centre for Medical Radiation Physics, University of Wollongong (Australia) for relative dosimetry in small megavoltage photon beams. These detectors, which differ in the topology of their 512 sensitive volumes, were originally fabricated on bulk p-type substrates. More recently, they have also been fabricated on epitaxial p-type substrates. In the literature, their performance has been individually characterized for quality assurance (QA) applications. The present study directly assessed and compared that of a MP512-bulk and that of a MP512-epitaxial in terms of radiation hardness, long-term stability, response linearity with dose, dose per pulse and angular dependence. Their measurements of output factors, off-axis ratios and percentage depth doses in square radiation fields collimated by the jaws and produced by 6 MV and 10 MV flattened photon beams were then benchmarked against those by commercially available detectors. The present investigation was aimed at establishing, from a medical physicist's perspective, how the bulk and epitaxial fabrication technologies would affect the implementation of the MP512s into a QA protocol. Based on results, the MP512-epitaxial would offer superior radiation hardness, long-term stability and achievable uniformity and reproducibility of the response across the 2D active area.

Keywords Dosimetry · 2D monolithic silicon-diode array detector · Epitaxial silicon · Megavoltage photon beam

Introduction

The Centre for Medical Radiation Physics (CMRP), University of Wollongong (Australia) has designed a range of silicon-detector prototypes dedicated to quality assurance (QA) applications in megavoltage (MV) photon beams delivered with medical linear accelerators (linacs) [1, 2]. Among these, it has proposed and characterized three 2D monolithic silicon-diode arrays (the MP512, the Duo and the Octa), different in the topology of their 512 diode-sensitive volumes (SVs) (Fig. 1).

The MP512 has SVs ($0.5 \times 0.5 \text{ mm}^2$) uniformly distributed over a square active area ($52 \times 52 \text{ mm}^2$) with a pitch of 2 mm. The Duo has SVs ($0.04 \times 0.8 \text{ mm}^2$) arranged along two linear arrays with a pitch of 0.2 mm to offer an improved resolution which would be of interest for measurements in small radiation fields ($\leq 1 \text{ cm}$ across). A compromise between the coarse resolution of the MP512 and the limited 2D dose map characterization of the Duo would be offered by the Octa. It has SVs ($0.04 \times 0.8 \text{ mm}^2$)

✉ A. B. Rosenfeld
anatoly@uow.edu.au

¹ Centre for Medical Radiation Physics (CMRP), University of Wollongong, Wollongong, Australia

² Department of Radiology, Faculty of Medicine, Mahidol University, Bangkok, Thailand

³ Illawarra Health and Medical Research Institute (IHMRI), Wollongong, Australia

⁴ Illawarra Cancer Care Centre (ICCC), Wollongong, Australia

⁵ Department of Medical Services, Lopburi Cancer Hospital, Lopburi, Thailand

⁶ SPA-BIT, Kiev, Ukraine

⁷ Peter MacCallum Cancer Centre, Melbourne, Australia

⁸ Sir Peter MacCallum Cancer Institute, University of Melbourne, Melbourne, Australia

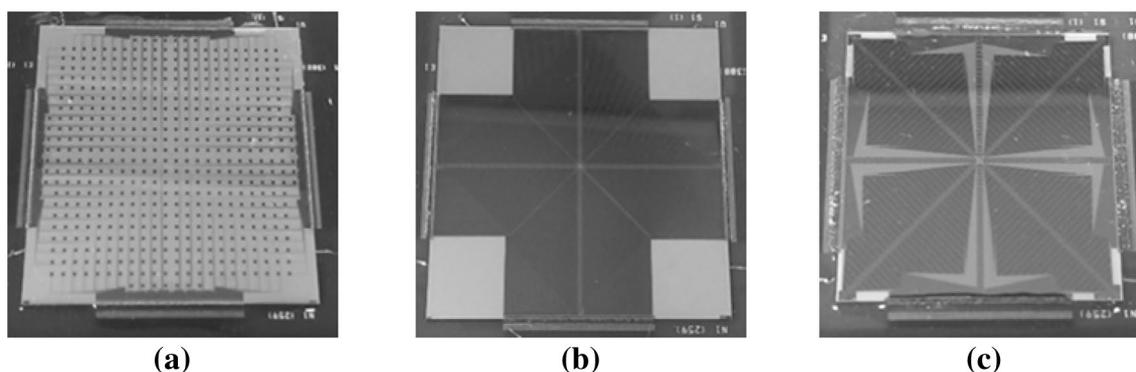


Fig. 1 2D monolithic silicon-diode array detectors proposed by the CMRP for QA in MV photon beams: **a** the MP512, **b** the Duo and **c** the Octa

arranged along four linear arrays at 45° relative to each other with a pitch of 0.3 mm along the vertical and horizontal arrays and of 0.43 mm along the two diagonals.

These devices, operated in passive mode (no external bias applied), have a high temporal resolution of the read-out electronics (pulse-by-pulse acquisition) [3] which makes them attractive for applications in dynamic stereotactic treatment modalities. They were devised for in-phantom measurements. As such, they are sandwiched between two 5 mm thick PMMA slabs, with the upper one having a small recess or air gap [4] on top of the SVs to minimize [5] the corrections required to account for the field size-dependent response of these silicon-based detectors in small MV photon beams [6].

The detectors were originally fabricated on a bulk p-type silicon-wafer Czochralski [7] substrate (resistivity of $10 \Omega\text{cm}$) and pre-irradiated to stabilize their response with accumulated dose [8]. More recently, the same devices have also been fabricated on a radiation-hard p-type epitaxial [9] layer (resistivity of $100 \Omega\text{cm}$), grown onto a thick heavily-doped silicon substrate (resistivity of $0.001 \Omega\text{cm}$). The thin active epitaxial layer has the required mechanical strength over large areas. These epitaxial devices may have improved radiation hardness and may not require pre-irradiation for sensitivity stabilization [10, 11].

In the literature, the performances of the MP512-bulk [12, 13], the MP512-epitaxial [14], the Duo-bulk [15], the Duo-epitaxial [16] and the Octa-epitaxial [17, 18] have been individually characterized for machine-specific and patient-specific QA. Machine QA describes procedures intended to verify the dosimetric parameters of a linac, such as its output factor. Patient QA, also referred to as pre-treatment QA, describes procedures to verify clinical plans. There is, however, a lack of a direct and thorough comparison of how the bulk and epitaxial fabrication technologies would affect the implementation of these devices into a QA protocol. Aiming at answering this question, the present study evaluated

and compared, from a medical physicist's perspective, the performance of a MP512-bulk and of a MP512-epitaxial.

Materials and methods

Dosimeters and participating facilities

Along with the MP512-bulk and the MP512-epitaxial prototypes, the present study considered as benchmark measurements, under the same experimental conditions, by multiple alternative detectors: GafchromicTM EBT3 films (Ashland Inc., USA), MOSkinTM detectors and three different ionization chambers (Table 1).

Films were scanned with a Microtrex ScanMaker i800 flatbed scanner using a 48-bit RGB and a resolution of 72 dpi. All films were pre- and post-scanned six times using only the last three optical density maps, maintaining a consistent orientation. The film analysis methodology was the same as that used by Aldosari et al. [12].

MOSkinTM are metal–oxide–semiconductor field-effect transistor (MOSFET)-based devices developed for real-time in vivo dose measurements. Their SV consists of a $0.55 \mu\text{m}$ thick SiO_2 layer, on top of a silicon substrate, mounted underneath a thin plastic layer with a uniform thickness of

Table 1 Description of benchmarking detectors considered for each test in the present study

Benchmarking detectors	Test
Films	Angular dependence, output factors (OFs), off-axis ratios (OARs)
MOSkin TM	OFs
CC13 chamber	Percentage depth dose (PDD)
Farmer chamber	Dose per pulse dependence
Markus chamber	PDD

0.07 mm. As such, they provide a skin-equivalent depth-dose when placed on a surface [19, 20].

The ionization chambers used were a CC13 (IBA Dosimetry, Germany), a Farmer chamber type NE2571A used with a UNIDOS electrometer (PTW, Germany) with a supply voltage of + 300 V, and a Markus chamber model N23343 (PTW, Germany).

Experimental measurements for radiation hardness investigation were performed at the Gamma Technology Research Irradiator (GATRI) facility at the Australian Nuclear Science and Technology Organisation (ANSTO, Lucas Heights, NSW, Australia). Investigations of long-term stability, response linearity with dose, dose per pulse dependence, angular dependence and measurements described in the “Clinical application” section were performed at the Illawarra Cancer Care Centre (ICCC, Wollongong, NSW, Australia) using a Varian Clinac® iX (Varian Medical System, Palo Alto, CA, USA) medical linac. The linac operated with a pulse frequency of 360 Hz and was calibrated to deliver 1 cGy/MU at d_{\max} in water at 100 cm source-to-surface distance (SSD).

Radiation hardness, long-term stability and response linearity with dose

Investigation of radiation hardness was performed by irradiating the MP512s with a dose rate 2.28 kGy/h using a Co-60 gamma source. The MP512-bulk was irradiated with a total water-equivalent dose of 80 kGy with response stability assessed after dose increments of 10 kGy. The MP512-epi was irradiated with a total water-equivalent dose of 140 kGy, with response stability assessed after dose increments of 20 kGy or 40 kGy. Response stability assessments were performed by irradiating the devices, at 1.5 cm depth in solid water phantom, 100 cm SSD, with a 10 cm side square field collimated by the jaws and produced by a 6 MV photon beam. Each measurement was repeated 5 times to minimize random uncertainties, and only the average response of the four central SVs was considered.

Investigation of long-term stability after pre-irradiation was performed by considering the response variation of the MP512s over 12 months. Assessments, made at 1 month intervals, were done by irradiating the devices, at 1.5 cm depth in solid water phantom, 100 cm SSD, with a 10 cm side square field collimated by the jaws and produced by a 6 MV photon beam. Accumulated total dose was 500 Gy, while each measurement had a delivered dose of 100 monitor units (MU) at 600 MU/min. Only the average response of the four central SVs was considered.

Investigation of response linearity was done in the range from 1 to 500 MU. The test was performed by irradiating the MP512s, at 1.5 cm depth in solid water phantom, 100 cm

SSD, with a 10 cm side square field collimated by the jaws and produced by 6 MV and by 10 MV photon beams.

Dose per pulse dependence

Investigation of the dose per pulse dependence of the response of the MP512s was performed by irradiating the devices, at 1.5 cm depth in solid water phantom, with a 10 cm side square field collimated by the jaws and produced by a 6 MV photon beam. The devices were irradiated by a fixed number of MU, changing the SSD in the range of 100–370 cm to change the dose per pulse at the detector location [12, 21]. Doses per pulse in the range from 0.01 to 0.34 mGy/pulse were considered. Each measurement was repeated 5 times to minimize random uncertainties.

The relative sensitivity S_{SSD} of the MP512s at any given SSD was defined as:

$$S_{SSD} = \frac{Q}{Q_{IC}} \quad (1)$$

with Q the average charge collected by their four central SVs and Q_{IC} the charge collected by the ionization chamber used as reference, at the same SSD (i.e. for the same dose per pulse). The dose per pulse dependence of the MP512s was defined as:

$$DPP_{dep} = \frac{S_{SSD}}{S_{SSD=ref}} \quad (2)$$

with $S_{SSD=ref}$ the sensitivity S_{SSD} at the reference dose per pulse of 0.278 mGy/pulse.

Angular dependence

Investigation of the angularly-dependent response was performed by irradiating the MP512s, lodged into a cylindrical PMMA phantom, with a 10 cm side square field collimated by the jaws and produced by 6 MV and 10 MV photon beams. The radiation-beam incidence angle θ was changed in the range from 0° to 180° in 10° steps, irradiating the MP512s at each step 5 times with 100 MU at 600 MU/min. Films were used as reference assuming their response is angular independent [22], although this has recently been disputed [23].

The investigation procedure, described also by Stansook et al. [24], starts with defining, for each SV of the MP512s, a calibration factor A as the ratio of their response, $MP(\theta)$, to the response of the film, EBT3(θ), in the same location:

$$A(\theta) = \frac{MP(\theta)}{EBT3(\theta)} \quad (3)$$

The angular response of each SV was then defined as:

$$C(\theta) = \frac{A(\theta)}{A(\theta=0^\circ)} \quad (4)$$

with $\theta = 0^\circ$ the incidence angle for which the beam was perpendicular to the 2D active surface of the MP512s. Only the average response of the four central SVs was considered.

Clinical application

As a clinical application, we considered measurements relevant to machine-specific QA, such as OFs, OARs and PDDs.

Prior to all measurements, the MP512s were aligned with respect to the machine central axis (CAX) by maximizing the response of their central SVs using the smallest available square field (0.5 cm side). Each measurement was repeated 3 times to minimize random uncertainties.

For OFs, the MP512s, at 10 cm depth in solid water phantom, 90 cm SSD, were irradiated with square fields in the range from 0.5 to 10 cm side collimated by the jaws and produced by 6 MV and 10 MV photon beams.

For OARs, the MP512s, at 10 cm depth in solid water phantom, 90 cm SSD, were irradiated with square fields in the range from 1 to 4 cm de collimated with the jaws and produced by a 6 MV photon beam. For a quantitative estimation of full-width half-maximum (FWHM) and penumbra width (taken as the distance between the 80% and the 20% isodose levels), all OARs were analysed with MATLAB® (MathWorks, Inc., Natick, MA, USA) using a shape-preserving interpolant function.

For PDDs, the MP512s were irradiated in a solid water phantom at depths in the range from 0.5 to 30 cm, 100 cm SSD, by a square field 10 cm side collimated by the jaws and produced by 6 MV and 10 MV photon beams. PDDs by the MP512s were benchmarked against those by a CC13 chamber for depths in the range from 1.5 to 3. cm and those by a Markus chamber for depths in the range from 0.5 to 10 cm. The known dose over-estimation by the Markus chamber was corrected for by following the Velkley and Rawlinson method [25, 26].

Results

Radiation hardness, long-term stability and response linearity with dose

Radiation hardness in terms of sensitivity degradation with accumulated dose is in Fig. 2 for both MP512s. Sensitivity is shown normalized to that at zero accumulated dose. Error bars, calculated as 1 standard deviation, did not exceed the symbol size. Sensitivity of the MP512-bulk was reduced to about 75% of the initial value after 10 kGy, that of the MP512-epitaxial was approximately 85% of the initial value after 80 kGy.

In terms of long-term stability, the variation in sensitivity was $\pm 10\%$ for the MP512-bulk, after up to 500 Gy

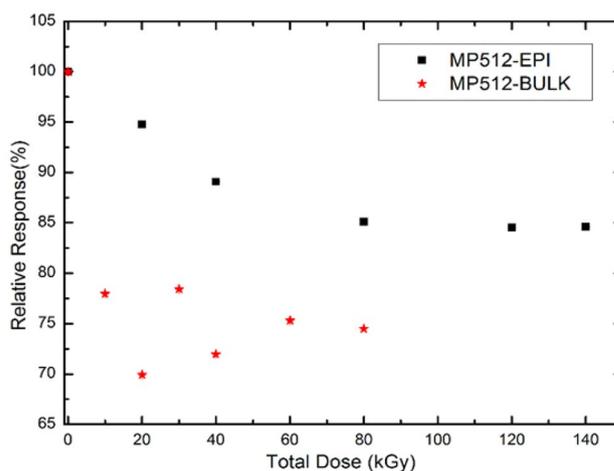


Fig. 2 Sensitivity degradation with accumulated dose of the MP512s. Response is shown normalized to that at zero dose. Sensitivity of the MP512-bulk was reduced to $\sim 75\%$ of the initial value after 10 kGy. Sensitivity of the MP512-epitaxial was reduced to $\sim 85\%$ of the initial value after 80 kGy

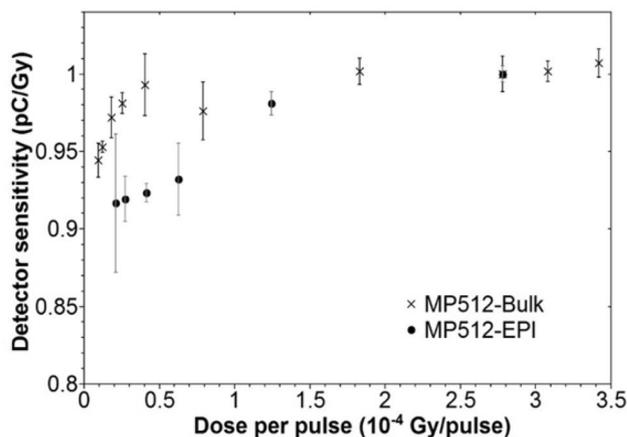


Fig. 3 Dose per pulse dependence of the MP512s. Response is shown normalized to that at 0.278 mGy/pulse. Maximum dose per pulse-dependence was $\sim 6\%$ at 0.01 mGy/pulse for the MP512-bulk. It was $\sim 8\%$ at 0.02 mGy/pulse for the MP512-epitaxial

delivered by a 6 MV photon beam over 12 months. It was within $\pm 0.9\%$, with 2 standard deviations being $\pm 0.03\%$, for the MP512-epitaxial.

The response of the MP512s was linear in the investigated dose range from 10 to 500 MU (adjusted regression coefficient $R^2 = 1.00 \pm 0.001$).

Dose per pulse dependence

The dose per pulse-dependence of the MP512s is in Fig. 3. Error bars are 1 standard deviation. Maximum dose per pulse-dependence was approximately 6% at 0.01 mGy/

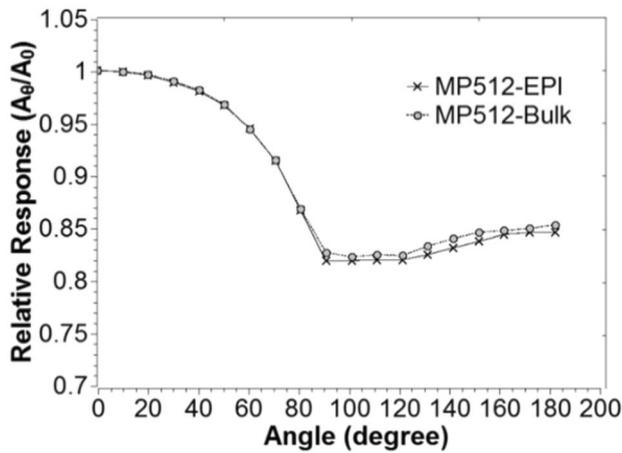


Fig. 4 6 MV beam: angularly-dependent response of the MP512s. 0° refers to incident-beam direction perpendicular to the 2D detector plane. Maximum sensitivity degradation was reached at incident-beam angle of 90°, i.e. beam direction parallel to the 2D detector plane

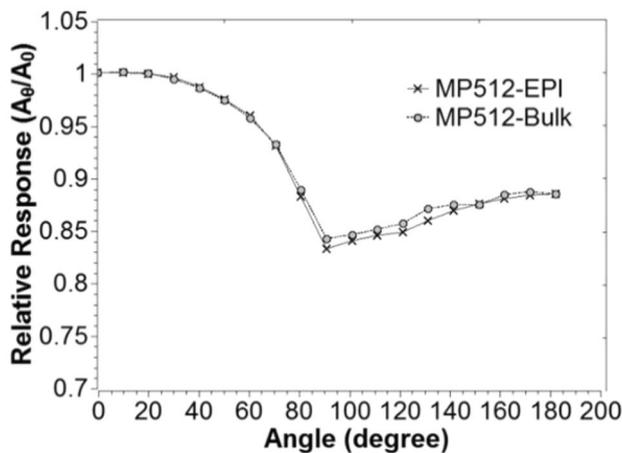


Fig. 5 10 MV photon beam: angularly-dependent response of the MP512s. Differences seen by comparing the angular dependence in a 6 MV and in a 10 MV beam are explained by beam quality-dependent perturbations to particle spectra introduced by SV and packaging

pulse, relative to 0.278 mGy/pulse, for the MP512-bulk. It was 8% at 0.02 mGy/pulse, relative to 0.278 mGy/pulse, for the MP512-epitaxial.

Angular dependence

The angularly-dependent response of the MP512s is in Fig. 4 (6 MV beam) and in Fig. 5 (10 MV beam). Error bars, calculated as 2 standard deviations, did not exceed the symbol size.

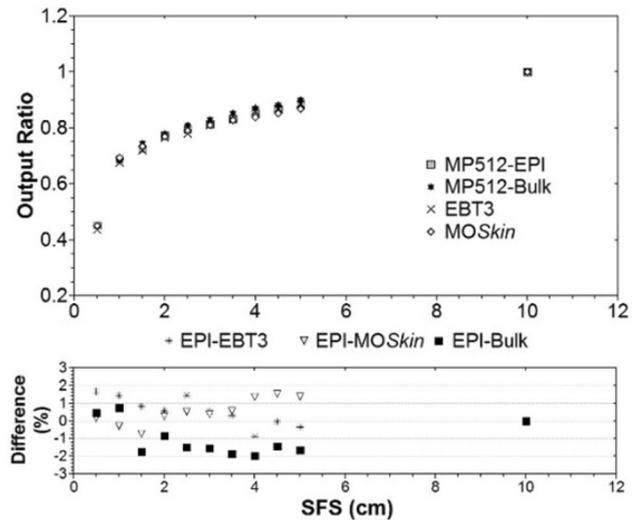


Fig. 6 6 MV beam: OFs by the MP512s, films and MOSkin™. Percentage differences are shown in the lower panel

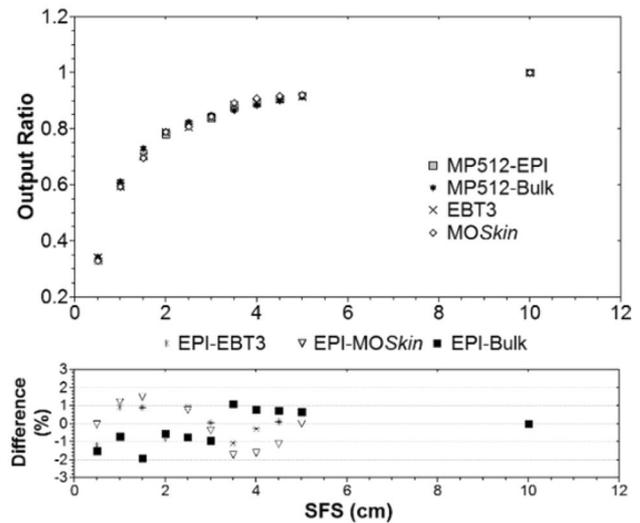


Fig. 7 10 MV beam: OFs by the MP512s, films and MOSkin™. Percentage differences are shown in the lower panel

Clinical application

OFs by the MP512s, films and MOSkin™ are in Fig. 6 (6 MV beam) and in Fig. 7 (10 MV beam). Percentage differences are shown in the lower panels.

A cross-plane OAR by the MP512-epitaxial and by film in a square field jaws-defined of 1 cm side is shown in Fig. 8 (6 MV beam). In all investigated fields, FWHMs of cross-plane OARs measured by the MP512-epitaxial agreed with those by films to within 1% in a 6 MV beam and to within 1.5% in a 10 MV beam. All penumbra widths agreed within 0.6 mm.

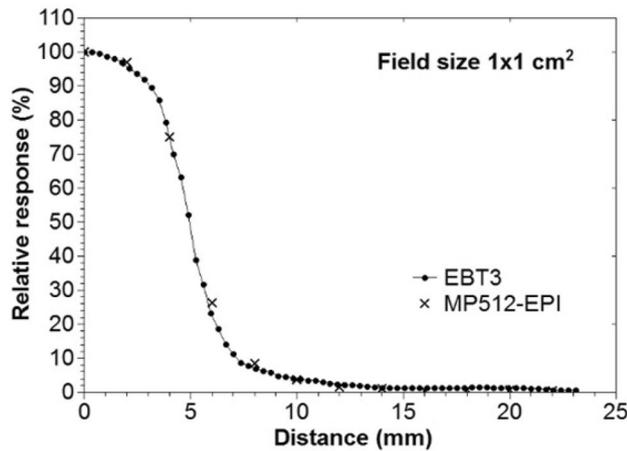


Fig. 8 6 MV beam: cross plane OAR in a 1 cm side square field by the MP512-epitaxial and by film

PDDs by the MP512s, Markus and CC13 chambers are in Fig. 9 (6 MV beam) and in Fig. 10 (10 MV beam). Differences between measurements by the MP512s and the chambers were within $\pm 2\%$ at all depths, for both beam energies investigated. Error bars, calculated as 2 standard deviations, do not exceed the symbol size.

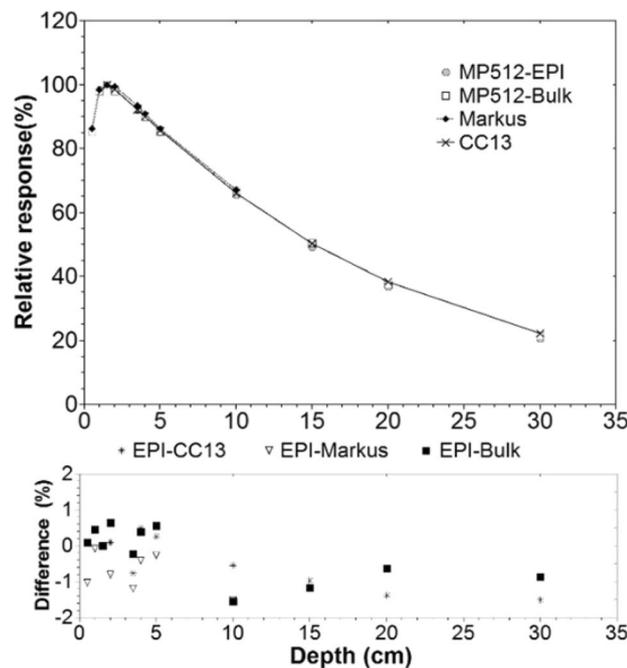


Fig. 9 6 MV beam: PDDs by the MP512s, Markus and CC13 chambers. Percentage differences are shown in the lower panel

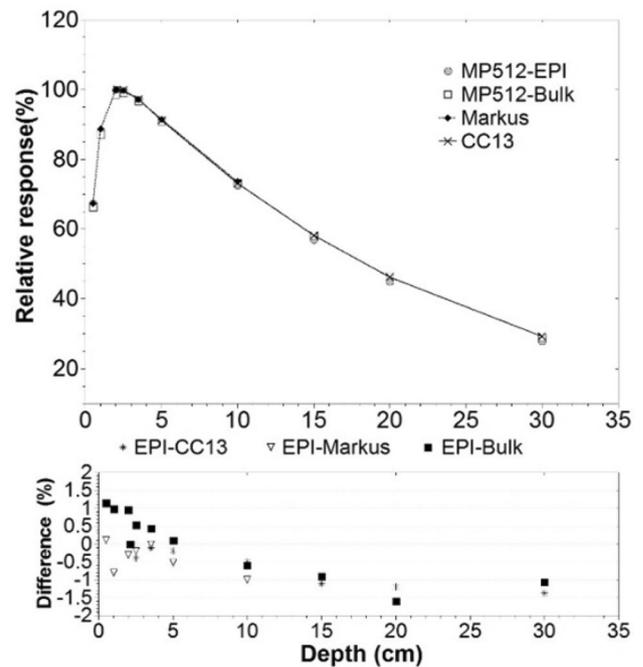


Fig. 10 10 MV beam: PDDs by the MP512s, Markus and CC13 chambers. Percentage differences are shown in the lower panel

Discussion

Radiation hardness, long-term stability and response linearity with dose

For a bulk device, pre-irradiation is required to stabilize its response with accumulated dose, at the cost of a reduced sensitivity [8]. In the present work, the sensitivity of the MP512-bulk was heavily reduced to close to 75% of the initial value and stabilized after irradiation with 20 kGy by a Co-60 gamma photon source, but with a residual sensitivity variation of approximately $\pm 5\%$ which would call for frequent recalibrations. The sensitivity of the MP512-epitaxial was stabilized within $\pm 3\%$ after 40 kGy and within $\pm 0.3\%$ after 80 kGy, demonstrating its superior radiation-hardness and making frequent recalibrations optional. Residual sensitivity was close to 85% of the initial value. These results can be complemented by those on the investigation of the long-term stability of the MP512s after pre-irradiation, adding to the superior performance of the MP512-epitaxial over the MP512-bulk.

The linear response of the MP512s in the investigated dose range from 10 to 500 MU agrees with previous investigations which have demonstrated that the MP512-bulk [12], the Octa-bulk and the Octa-epitaxial [27] were linear in the dose range 50–500 MU. These results suggest that both a bulk and an epitaxial substrate would in

principle offer an equivalent performance in terms of response linearity with delivered dose.

Dose per pulse dependence

The dose per pulse of the order of 10^2 Gy/s under which the detector is operated is much different than the average dose to water delivered by medical linacs of the order of 4 Gy/min at d_{\max} [1, 28]. For QA applications, the dose per pulse varies with depth in water, across the radiation field, due to introduction of beam attenuators [29] and, if flattening filter free photon beams are used, also in the central axis region of a radiation field [30]. The dose per pulse dependence of the response of silicon-based detectors is well-known, with a decrease in sensitivity expected with decreased dose per pulse, as first reported by Rikner and Grusell [31]. This dependence affects measurement accuracy and would call for a correction.

Previous studies have investigated the dose per pulse dependence of the MP512, Duo and Octa in a 6 MV beam. The MP512-bulk had a maximum sensitivity degradation of approximately 5% in the range from 0.009 to 0.34 mGy/pulse with respect to 0.278 mGy/pulse [12]. The Duo-bulk had sensitivity degradation within 23% at 0.021 mGy/pulse with respect to 0.278 mGy/pulse [15]. The non-preirradiated Octa-epitaxial had a maximum sensitivity degradation of close to 26% at 0.021 mGy/pulse relative to 0.278 mGy/pulse [32].

In the present study, the maximum sensitivity degradations of approximately 6%, MP512-bulk, and 8% MP512-epitaxial, found was of the same order of magnitude between the two devices. The degradation was however significantly smaller than that reported by investigations on the Duo and on the Octa, a result which would merit further investigation. The larger relative sensitivity degradation of the MP512-epitaxial over the MP512-bulk can be explained by the fact that the dose per pulse dependence decreases by decreasing the resistivity of the silicon active substrate, or by reducing the minority carrier lifetime by pre-irradiation [11, 33].

Angular dependence

The angularly-dependent response of a silicon detector is mainly explained in terms of anisotropy in its materials and assembly [34].

In a previous investigation [32], the Octa-bulk had a maximum angular dependence of 30% in the case of a 6 MV beam. The Octa-epitaxial had a maximum angular dependence of 23% in the case of a 6 MV beam and of 20% in the case of a 10 MV beam. It was also reported that the MP512-bulk [24] had a maximum angular dependence

of $18.5\% \pm 0.5\%$ in the case of a 6 MV beam and of $15.5\% \pm 0.5\%$ in the case of a 10 MV beam.

In the present study, results for the MP512-epitaxial were within $\pm 2\%$ of those for the MP512-bulk [24] at all angles. In all cases, maxima were reached at incident beam angle of 90° i.e. when the beam direction was parallel to the 2D detector plane. In the range from 0° to 90° , angular dependence increases owing to increasing beam attenuation by the silicon. From 90° to 180° , angular dependence decreases for the opposite reason. In this case, lower relative values are explained by additional attenuation owing to the detector packaging. The differences seen by comparing the angular dependence in a 6 MV beam with that in a 10 MV beam are explained by beam quality-dependent perturbations to the particle spectra introduced by the SV and its packaging [6].

For application in arc radiotherapy QA, the angularly-dependent response of a detector such as the MP512 can be mitigated by corrections [14, 24], provided the radiation-beam incidence angle is known at any time. Alternatively, the 2D active surface could be maintained always perpendicular to the incident beam by using a suitable rotating phantom.

These results, supported by those of a previous investigation [32], suggest that the MP512-bulk and the MP512-epitaxial are affected by a comparable angularly-dependent response. To minimize uncertainties in the reported dose measurements, however, the devices would call for correction factors to be measured individually, for each field size and beam quality considered.

Clinical application

OFs by the MP512s agreed within $\pm 2\%$ with those by films and *MOSkin*TM, for all square fields investigated in the range 0.5–10 cm side, for both 6 MV and 10 MV beams.

Considered cross-plane OARs in square fields defined by the jaws in the range 1–4 cm with a 6 MV beam, it was found that FWHMs by the MP512-epitaxial agreed within $\pm 1\%$ with those by films, while penumbra widths agreed within 0.6 mm. These results were consistent with those by the MP512-bulk reported in a previous investigation, in which discrepancies with respect to results by films were within $\pm 1.2\%$ [12]. In the same radiation fields with a 10 MV beam, FWHMs by the MP512-epitaxial agreed within $\pm 1.6\%$ with those by films, and penumbra widths agreed within 0.6 mm.

Considering PDDs, differences between measurements by the MP512s and the chambers were within $\pm 2\%$ at all depths, for both beam energies investigated. Difference

between measurements by the MP512-bulk and the MP512-epitaxial were always within $\pm 2\%$.

Conclusions

The present study assessed and compared the performance of two prototype detectors, a MP512-bulk and a MP512-epitaxial, in the context of QA applications in megavoltage photon beams delivered by medical linear accelerators.

Experimentally, both MP512s showed good linearity with delivered dose. However, the MP512-epitaxial demonstrated a superior radiation hardness and long-term stability of the response, suggesting pre-irradiation may not be necessary and frequent recalibrations would be redundant. It was then highlighted that both the MP512s were affected by a dose per pulse and angular dependence of a similar magnitude, requiring suitable corrections to be assessed individually. Their performance in terms of typical machine-specific QA measurements, such as OFs, OARs and PDD, were also of comparable accuracy when benchmarked with commercially available detectors.

Based on these results, supported by those reported by previous investigations [27, 32, 35], our conclusion is that, from a medical physicist's perspective, the MP512-epitaxial would be the candidate of choice as a QA tool owing to superior radiation hardness, long-term stability and achievable uniformity and reproducibility of the response of the SVs across a large 2D active area. We also expect the same conclusion to apply to similar devices (Duo-bulk, Duo-epitaxial and Octa-bulk, Octa-epitaxial), which differ from the MP512 only in the topology of the SVs.

Acknowledgements Nauljun Stansook was supported by a faculty of Medicine Ramathibodi Hospital (Mahidol University, Bangkok, Thailand). We would like to acknowledge the Gross Foundation (Melbourne, Australia) for financial support. The authors are also grateful to Dr. Justin Davies at the GATRI facility (ANSTO, Lucas Heights, Australia).

Funding This study was funded by the National Health and Medical Research Council of Australia with the Project Grant No. APP1030159.

Compliance with ethical standards

Conflict of interest The authors declare they have no conflicts of interest.

Research involving human and animal participants This article does not contain any studies with human participants or animals performed by any of the authors.

References

- Rosenfeld AB (2007) Electronic dosimetry in radiation therapy. *Radiat Meas* 41:S134–S153
- Rosenfeld AB (2011) Advanced semiconductor dosimetry in radiation therapy. In: Rozenfeld A (eds) Concepts and trends in medical radiation dosimetry, vol. 1345. American Institute of Physics, Melville, NY, pp. 48–74
- Fuduli I, Newall MK, Espinoza A, Porumb CS, Carolan MG, Lerch MLF, Metcalfe P, Rosenfeld AB, Petasecca M (2014) Multi-channel data acquisition system comparison for quality assurance in external beam radiation therapy. *Radiat Meas* 71:338–341
- Charles PH, Crowe SB, Kairn T, Knight RT, Hill B, Kenny J, Langton CM, Trapp JV (2013) Monte Carlo-based diode design for correction-less small field dosimetry. *Phys Med Biol* 58(13):4501–4512
- Utisarn K, Alrowaili ZA, Stansook N, Lerch MLF, Petasecca M, Carolan MG, Rosenfeld AB (2017) Optimisation of output factor measurements using the Magic Plate 512 silicon dosimeter array in small megavoltage photon fields. *J Phys Conf Ser* 777:012022
- Andreo P (2018) The physics of small megavoltage photon beam dosimetry. *Radiother Oncol* 126(2):205–213
- Czocharlski J (1918) Ein neues Verfahren zur Messung der Kristallisationsgeschwindigkeit der Metalle. *Zeitschrift für Phys Chemie* 92U(1):219–221
- Rikner G, Grusell E (1987) General specifications for semiconductors for use in radiation dosimetry. *Phys Med Biol* 32(9):1109–1117
- Sze SM, Ng KK (2007) Physics of semiconductor devices, 3rd edn. Wiley, New York
- Bruzzi M, Bucciolini M, Casati M, Menichelli D, Talamonti C, Piemonte C, Svensson BG (2007) Epitaxial silicon devices for dosimetry applications. *Appl Phys Lett* 90(17):17–19
- Bruzzi M (2016) Novel silicon devices for radiation therapy monitoring. *Nucl Instrum Methods Phys Res Sect A* 809:105–112
- Aldosari AH, Petasecca M, Espinoza A, Newall MK, Fuduli I, Porumb CS, AlShaikh S, Alrowaili ZA, Weaver MR, Metcalfe P, Carolan MG, Lerch MLF, Perevertaylo V, Rosenfeld AB (2014) A two dimensional silicon detectors array for quality assurance in stereotactic radiotherapy: MagicPlate-512. *Med Phys* 41(9):091707
- Petasecca M, Newall MK, Booth JT, Duncan M, Aldosari AH, Fuduli I, Espinoza A, Porumb CS, Guatelli S, Metcalfe P, Colvill E, Cammarano D, Carolan MG, Oborn BM, Lerch MLF, Perevertaylo V, Keall PJ, Rosenfeld AB (2015) MagicPlate-512: a 2D silicon detector array for quality assurance of stereotactic motion adaptive radiotherapy. *Med Phys* 42(6):2992–3004
- Duncan M, Newall MK, Caillet V, Booth JT, Keall PJ, Lerch MLF, Perevertaylo V, Rosenfeld AB, Petasecca M (2018) Real-time high spatial resolution dose verification in stereotactic motion adaptive arc radiotherapy. *J Appl Clin Med Phys* 19(4):173–184
- Al Shukaili K, Petasecca M, Newall MK, Espinoza A, Perevertaylo V, Corde S, Lerch MLF, Rosenfeld AB (2017) A 2D silicon detector array for quality assurance in small field dosimetry: DUO. *Med Phys* 44(2):628–636
- Al Shukaili K, Corde S, Petasecca M, Perevertaylo V, Lerch MLF, Jackson M, Rosenfeld AB (2018) Characterization of ELEKTA SRS cone collimator using high spatial resolution monolithic silicon detector array. *J Appl Clin Med Phys* 19(4):114–124
- Biasi G, Petasecca M, Guatelli S, Hardcastle N, Carolan M, Perevertaylo V, Kron T, Rosenfeld AB (2018) A novel high-resolution 2D silicon array detector for small field dosimetry with FFF photon beams. *Phys Medica* 45:117–126
- Biasi G, Petasecca M, Guatelli S, Martin EA, Grogan G, Hug B, Lane J, Perevertaylo V, Kron T, Rosenfeld AB (2018) CyberKnife® fixed cone and Iris™ defined small radiation fields: assessment with a high-resolution solid-state detector array. *J Appl Clin Med Phys* 19(5):547–557
- Kwan IS, Rosenfeld AB, Qi ZY, Wilkinson D, Lerch MLF, Cutajar DL, Safavi-Naeini M, Butson MJ, Bucci J, Chin Y, Perevertaylo V

- (2008) Skin dosimetry with new MOSFET detectors. *Radiat Meas* 43(2–6):929–932
20. Metcalfe P, Quinn A, Loo K, Lerch MLF, Petasecca M, Wong JHD, Hardcastle N, Carolan MG, McNamara J, Cutajar DL, Fuduli I, Espinoza A, Porumb CS, Rosenfeld AB (2013) Review of four novel dosimeters developed for use in radiotherapy. *J Phys Conf Ser* 444:012008
 21. Saini AS, Zhu TC (2004) Dose rate and SDD dependence of commercially available diode detectors. *Med Phys* 31(4):914–924
 22. Huet C, Moignier C, Fontaine J, Clairand I (2014) Characterization of the gafchromic EBT3 films for dose distribution measurements in stereotactic radiotherapy. *Radiat Meas* 71:364–368
 23. Yuasa Y, Kawamura S, Shiinoki T, Uehara T, Koike M, Kanzaki R, Hanazawa H, Takahashi S, Shibuya K (2016) Evaluation of the incident directional dependence of radiochromic film by use of Monte Carlo simulation and measurement. *Radiol Phys Technol* 9(2):227–232
 24. Stansook N, Utitsarn K, Petasecca M, Newall MK, Duncan M, Nitschke K, Carolan MG, Metcalfe P, Lerch MLF, Perevertaylo V, Tomé WA, Rosenfeld AB (2017) Technical note: angular dependence of a 2D monolithic silicon diode array for small field dosimetry. *Med Phys* 44(8):4313–4321
 25. Gerbi BJ, Khan FM (1990) Measurement of dose in the buildup region using fixed-separation plane-parallel ionization chambers. *Med Phys* 17(1):17–26
 26. Mellenberg DE (1990) Determination of build-up region over-response corrections for a Markus-type chamber. *Med Phys* 17(6):1041–1044
 27. Biasi G, Davis J, Petasecca M, Guatelli S, Perevertaylo V, Kron T, Rosenfeld AB (2018) On monolithic silicon array detectors for small-field photon beam dosimetry. *IEEE Trans Nucl Sci* 65(9):2640–2649
 28. Jursinic PA (2013) Dependence of diode sensitivity on the pulse rate of delivered radiation. *Med Phys* 40(2):021720
 29. Shi J, Simon WE, Zhu TC (2003) Modeling the instantaneous dose rate dependence of radiation diode detectors. *Med Phys* 30(9):2509–2519
 30. Budgell G, Brown K, Cashmore J, Duane S, Frame J, Hardy M, Paynter D, Thomas R (2016) IPEM topical report 1: guidance on implementing flattening filter free (FFF) radiotherapy. *Phys Med Biol* 61(23):8360–8394
 31. Rikner G, Grusell E (1983) Effects of radiation damage on p-type silicon detectors. *Phys Med Biol* 28(11):1261–1267
 32. Biasi G, Hardcastle N, Petasecca M, Guatelli S, Perevertaylo V, Kron T, Rosenfeld AB (2019) On the instantaneous dose rate and angular dependence of monolithic silicon array detectors. *IEEE Trans Nucl Sci* 66(1):519–527
 33. Grusell E, Rikner G (1993) Linearity with dose rate of low resistivity p-type silicon semiconductor detectors. *Phys Med Biol* 38(6):785
 34. Jursinic PA, Sharma R, Reuter J (2010) MapCHECK used for rotational IMRT measurements: step-and-shoot, Tomotherapy, RapidArc. *Med Phys* 37(6):2837–2846
 35. Aldosari AH, Espinoza A, Robinson D, Fuduli I, Porumb CS, AlShaikh S, Carolan MG, Lerch MLF, Perevertaylo V, Rosenfeld AB, Petasecca M (2013) Characterization of an innovative p-type epitaxial diode for dosimetry in modern external beam radiotherapy. *IEEE Trans Nucl Sci* 60(6):4705–4712

Publisher's Note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.