



Computer assisted orthopaedic surgery: Past, present and future

Frederic Picard^{a,b,*}, Angela Helen Deakin^a, Philip E. Riches^b, Kamal Deep^a, Joseph Baines^a

^a Golden Jubilee National Hospital, Agamemnon Street, Clydebank, G81 4DY, UK

^b Department of Biomedical Engineering, University of Strathclyde, Wolfson Centre, 106 Rottenrow, Glasgow, G4 0NW, UK

ARTICLE INFO

Article history:

Received 11 June 2019

Accepted 23 August 2019

Keywords:

Computer assisted orthopaedic surgery

Navigation

Robotics

Knee surgery

Imaging technology

Registration

Review

ABSTRACT

Computer technology is ubiquitous and relied upon in virtually all professional activities including neurosurgery, which is why it is surprising that it is not the case for orthopaedic surgery with fewer than 5% of surgeons using available computer technology in their procedures. In this review, we explore the evolution and background of Computer Assisted Orthopaedic Surgery (CAOS), delving into the basic principles behind the technology and the changes in the discussion on the subject throughout the years and the impact these discussions had on the field. We found evidence that industry had an important role in driving the discussion at least in knee arthroplasty—a leading field of CAOS—with the ratio between patents and publications increased from approximately 1:10 in 2004 to almost 1:3 in 2014. The adoption of CAOS is largely restrained by economics and ergonomics with sceptics challenging the accuracy and precision of navigation during the early years of CAOS moving to patient functional improvements and long term survivorship. Nevertheless, the future of CAOS remains positive with the prospect of new technologies such as improvements in image-guided surgery, enhanced navigation systems, robotics and artificial intelligence.

© 2019 IPEM. Published by Elsevier Ltd. All rights reserved.

1. Introduction

Computer technology is ubiquitous and relied upon in virtually all professional activities. Contrast this with orthopaedic surgical practice, where fewer than 5% of surgeons in the USA, Europe and Asia are using computer-assisted technologies routinely [1]. Although first introduced in the 1990s [1], computer-assisted technology in orthopaedic surgery, or more simply Computer Assisted Orthopaedic Surgery (CAOS), is still not commonplace compared to un-assisted, conventional orthopaedic surgery.

It is currently predicted that a \$1000 computer will be able to carry out the same number of calculations per second as the human brain by 2025 [2]. Will this mean that computerised systems will exceed surgeons' skills, not only diagnosing and assessing patients but, more importantly, in surgical accuracy and precision even in complicated cases such as complex trauma or reconstructive surgery? According to Moravec [3], contrary to traditional assumptions, high level reasoning requires relatively little computer power, whereas low-level sensorimotor skills require enormous computational resources. Therefore CAS may solve some of the surgeon's task but not all. Furthermore, is a demand for enhanced accuracy warranted? After all, one of most commonly discussed issues with CAOS is the impact that accuracy of computer-

assisted surgery has had on the outcomes of surgical procedures [4].

It may be considered somewhat surprising therefore, at a time of incredible technological progress, with the advent of virtual and augmented reality, big data analysis and artificial intelligence, that the computer still struggles to make its way into all orthopaedic theatres of the world. This raises important questions regarding the paradoxical apathy towards the possible improvements of patient outcome through the use of CAOS and the impact of CAOS on the mainstream principles and concepts in the orthopaedic forum.

In this article, we begin by outlining some of the definitions related to CAOS and review general principles and key advances in today's state-of-the-art CAOS. Thereafter, we describe CAOS historical background before delving into the impact that CAOS has had on the general "orthopaedic forum" and the way it approaches diagnostic and therapeutic guidelines, focussing the discussion on knee and hip replacement surgeries. Finally, we speculate on future directions and offer our conclusions.

2. A few definitions

Computer-assisted orthopaedic surgery (CAOS) includes all kinds of computerised tools, devices and instrumentations, such as robotic assisted or navigation technology, but also patient-specific instrumentation and even sensors. These are all used for, not only assisting the surgeon in augmenting surgical procedures, but

* Corresponding author.

E-mail address: frederic.picard@gnh.scot.nhs.uk (F. Picard).

also for providing hitherto unavailable quantitative data, measuring data not seen and sometimes not known by the surgeon which could help fine tune the surgery to an individual profile.

Three major components are common to any of these systems, as described in Zheng and Nolte's excellent review paper published in 2015 [5]:

- The first component is a *therapeutic object* which is the target of treatment. For instance, it can be a joint to replace or a tumour to resect in a specific patient.
- The second component is a *virtual object* which is the virtual representation of any object that the surgeon wants to implant (e.g., joint replacement) or resect (e.g., oncologic lesion) at any place of the patient's body.
- The third component is a *navigator link* between these two objects.

CAOS technology offers a multitude of devices and complex mathematical algorithms to manipulate virtually, not only the patient's anatomy, but also any surgical tools and implants in real time. For instance, a 3-dimensional CT image of a patient's hip can be seen and assessed virtually on a monitor, whilst at the same time overlaying a perfectly fitting cup for simulation purposes [6,7]. During the preoperative planning phase, the *navigation link* is the software programme enabling virtual manipulation of both the *therapeutic and virtual object(s)* (hip anatomy and cup replacement). This concept of virtual simulation is applicable to any system using image-guided technology either preoperatively or intraoperatively [8]. Intraoperatively, the *navigation link*, such as a navigator or robot, allows the actual tracked object, e.g., a cutting tool, to be guided into the matched anatomy. This model also works for image-free computer-assistance following intraoperative data collection and registration of the "surgeon-defined anatomy", which generates the *therapeutic object* [9,10].

3. General principles

All CAOS systems positioned near patients for surgical assistance follow four outline steps: Setup, Registration, Planning and Execution (Fig. 1). The order of these stages depends on whether an a priori image is part of the workflow and used for planning. If so, the order is Planning, Setup, Registration, Execution. However, if planning is interoperative, the order of the steps is as before.

- *Set-up* refers to the initialisation process where the important objects are placed and identified within the operation space:

trackers are fixed to suitable bony structures of the patient, and the data-capturing object(s) (e.g., camera and/or robot) are placed in theatre around the patient.

- *Registration* refers to prescribing the coordinates, in system-space, of important anatomical landmarks, and either registering them to a prior 3d image, or using them to define the therapeutic object (i.e., anatomical structure) directly.
- In *Planning* the intended aim of the procedure is prescribed. In CAOS, this is the definition of the ideal position of the *virtual object* within the *therapeutic object*. This stage could be done either pre-operatively using medical imaging technology or intra-operatively using image-free navigation or intraoperative imaging technology.
- *Execution* is self-explanatory. In CAOS, the level of agency for the surgeon varies depending on the type of system. In navigation technology, the surgeon is in full control of the surgery allowing for deviation from the initial plan whereas in robotic technology, the surgeon follows a presurgical plan typically without deviation.

Indeed, it all starts from the patient's anatomy, which is analysed and assessed using imaging technology either pre-operatively (red arrow) or intra-operatively (green arrow). From there, a series of complex algorithms provide the surgeon and surgical team a 3-D reconstruction of the *therapeutic object* (for instance, the hip) and overlay it in real time into a *virtual object* (for instance a cup replacement). The surgical team or the surgeon can manipulate, in real time, both the *therapeutic object* and the *virtual object* in order to plan the surgery. This can be done pre-operatively, or intra-operatively [5]. Once the planning is completed, then the surgeon or the surgical team can upload the planning and consequently navigate or robotically assist the planned surgery.

The CT-free or image-free navigation concept removes the image processing planning and matching so the surgeon and the surgical team are building up intra-operatively the *therapeutic object* (i.e., an abstract of the patient's anatomy) directly from the patient's anatomy (green arrow) (see Fig. 1). The built frame of reference is assembled virtually with a series of relevant anatomical or kinematical landmarks to create the *therapeutic object*. Then, any calibrated tools (*virtual object*) are superimposed to the created therapeutic object to execute intraoperative plan [10,11].

Whatever computer-assisted system is used, *registration* is one of the core principles and a compulsory process that any CAOS system requires to work. Accuracy and precision are at the centre of the CAOS project with the promise to reduce outliers and improve

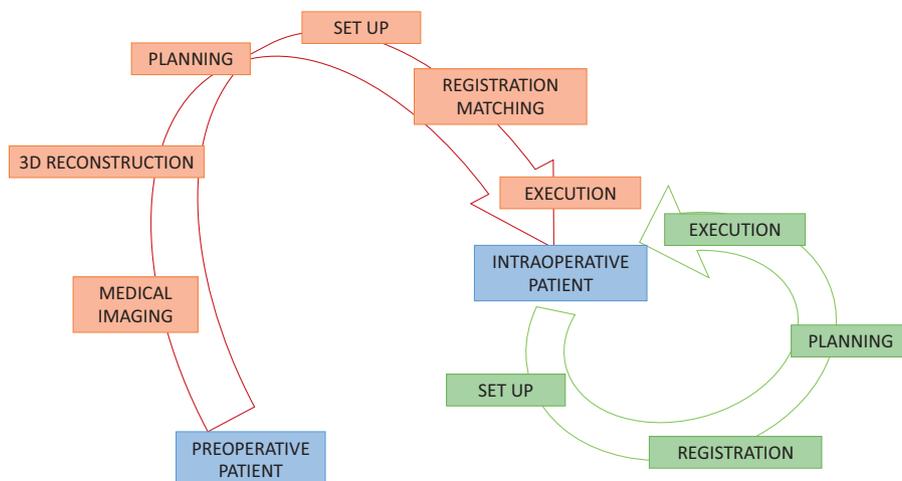


Figure 1. General principles: Image-guided (in red on left hand side) versus image-free (in green on right hand side) CAOS systems. The image-guided workflow has the planning carried out pre-operatively.

functional and clinical outcomes and the quality of registration is fundamental to reach trueness and precision in CAOS [4].

Any registration technique is basically trying to either build a patient-specific frame of reference as an abstract of the patient's anatomy [e.g., image-free navigation] or to collect enough anatomical landmarks to match the pre-operative or the intra-operative imaging model(s). Any registration process requires DRB (digital rigid bodies) which need to be rigidly fixed to a bony structure in order to capture either an anatomical abstract [e.g., image-free navigation] or a complex anatomical model [e.g., image-based navigation]. It is important to mention that robotic-assisted technology also relies greatly on the registration technique and more so than navigation because the surgical tasks are performed through robotic tools and not by surgical hands [1,5,12].

In image based systems the ultimate goal of registration is to fuse or overlap the patient's anatomy with any sort of medical imaging modalities. Several kinds of imaging can be used, such as CT scans, MRI scans or combined [13] and even ultrasound [14]. On the other hand, intra-operative registration of intraoperative anatomical landmarks can also be matched to statistical shape models using generic bony shapes or anatomical atlases [15].

The complex mathematical algorithms applied to registration processes are mainly divided in four different modalities:

- Fiducial-based registration: this has not been very well accepted because it involves the use of additional surgical steps prior to the main one with the risk of local inflammation, infection and pain [16].
- Landmark-based registration: which has been favoured because it requires only the use of a calibrated probe or pointer intra-operatively, defining relevant anatomical landmarks. However, this process can occasionally be tedious and time-consuming [17].
- Shape-based registration: this is very close to so-called “bone morphing”, which requires data collection of “painted” surfaces of the bone and using mesh linking all these points to aggregate them all and build up 3-D model surface(s), which could then be matched to the pre-operative 3-D image reconstruction [18].
- Finally, Intensity-based registration used mainly in fluoroscopy registration. This last technique allows the reduction of radiation dose during surgery because after completing registration and matching it is not necessary to take any further image intensifier shots during the surgical procedure [19]. This last modality is mainly used in spine and trauma surgery.

This registration process requires precalibrated tools, such as probe or pointer with various forms and designs all utilised to collect landmarks for the above registration modalities [9]. The surgical calibrated probe is to intra-operative registration, what the computer mouse is to the computer-assisted planning.

4. Key advances and state-of-the-art in the field of CAOS at the present

CAOS systems can be divided into three different categories using potentially three different registration technologies [49]:

- Active systems are autonomous, e.g., Robodoc® [50];
- Semi-active systems utilise handheld or controlled forced robotic assisted devices, e.g., the MAKO® [46,51]; and
- Passive systems only provide guiding information but no direct action, e.g., OrthoPilot® (Aesculap/BBraun, Germany) [52].

All three categories of systems can use different registration technologies:

- Pre-operative image technology, such as CT scans, MRIs, to assess specifically the therapeutic object (e.g., MAKO®) [53,54].

- Intra-operative medical imaging, such as fluoroscopy (image intensifier) commonly used in trauma and spine surgery, e.g., FluoNav-Medtronic® (Surgical Navigation Technology, USA) [55].
- CT-free or image-free technology, also called “surgeon defined anatomy”, e.g., NavioPFS® [56].

Any combination between these three categories and three modalities is theoretically possible. In reality, there are still a few combinations which are not on the market. To our knowledge, there are no active robots using only fluoro-based registration nor any combined with image-free technology, otherwise the other combinations are already on the market.

5. Background and history

If the computer had existed at the beginning of the 20th Century, computer-assisted surgery would have been invented by Clarke and Horsley in 1906 [20]. These two researchers published and patented in 1908 a stereotactic frame and instrument for reproducible and systematic “navigation” in the monkey cerebellum based on external visible landmarks. This very same concept was used later with orthogonal X-rays by E. Spiegel in 1947 [21]. Much later in 1985, the PUMA robot (Programmable Universal Machine for Assembly) was coupled with a stereotactic frame and was applied to neurosurgery [22]. Robotic-guided surgery based on pre-operative 3D computer tomodensitometry planning was FDA approved in 1987 (NeuroMate, Integrated Surgical Systems, Inc.) [23], eighty years after Clarke and Horsley's original article. Neurosurgeons embraced the technology, keen to develop safe options to reduce brain damage caused by invasive surgery during stereotactic surgery. In 2004, McBeth et al. stated “*The introduction of robotically assisted surgery has provided surgeons with improved ergonomics and enhanced visualization, dexterity, and haptic capabilities*” [24]. In the late eighties, ENT surgeons used image-guided technology to plan and guide complex reconstruction, but this did not disrupt the field as it has done in neurosurgery [25,26]. For many years, neurosurgeons and orthopaedists have been performing both spine surgery. New developments in spine instrumentation, such as transpedicular screw fixation, gave rise to computer assisted technology in the field. Teams spread across the world in Switzerland (Bern), the USA (Detroit, Memphis) and France (Grenoble) simultaneously, developing technology to guide pedicle screw surgery [12].

Since Hounfield's [27] and Lauterbur's [28] initial works on CT and MRI technology respectively, tremendous progress has been made in not only new diagnostic tools but also in computer-assisted 3D reconstruction [29]. Mathematical algorithms combined with new hardware, facilitated patient-specific planning, matching, modelling, intraoperative registration and intraoperative guidance [1]. Computer-assisted design (CAD) and computer-assisted manufacturing (CAM), in the orthopaedic world, expedited “custom-made implants”. Developed in the early 1980s by Aldinger et al. [30] to design perfectly fitting, patient-specific femoral stem implants [30], this concept is still used routinely for complex joint reconstructions in hip revisions, or for oncology cases during which surgeons perform large skeletal resections [31].

Instead of creating bespoke implants to match the patient's anatomy, the concept of machining the patient's anatomy to facilitate using standard implant sizes was advanced. This development produced the first ever computer-assisted technology system in orthopaedics, Robodoc® (Curexo Technology, Fremont, CA), first used on humans in 1992 [32]. Robodoc® was an “active robot” or “autonomous robotic device” which excluded the surgeon from the task of rasping the femur to enlarge the intramedullary canal to fit the femoral stem in total hip replacement (THR). Following this

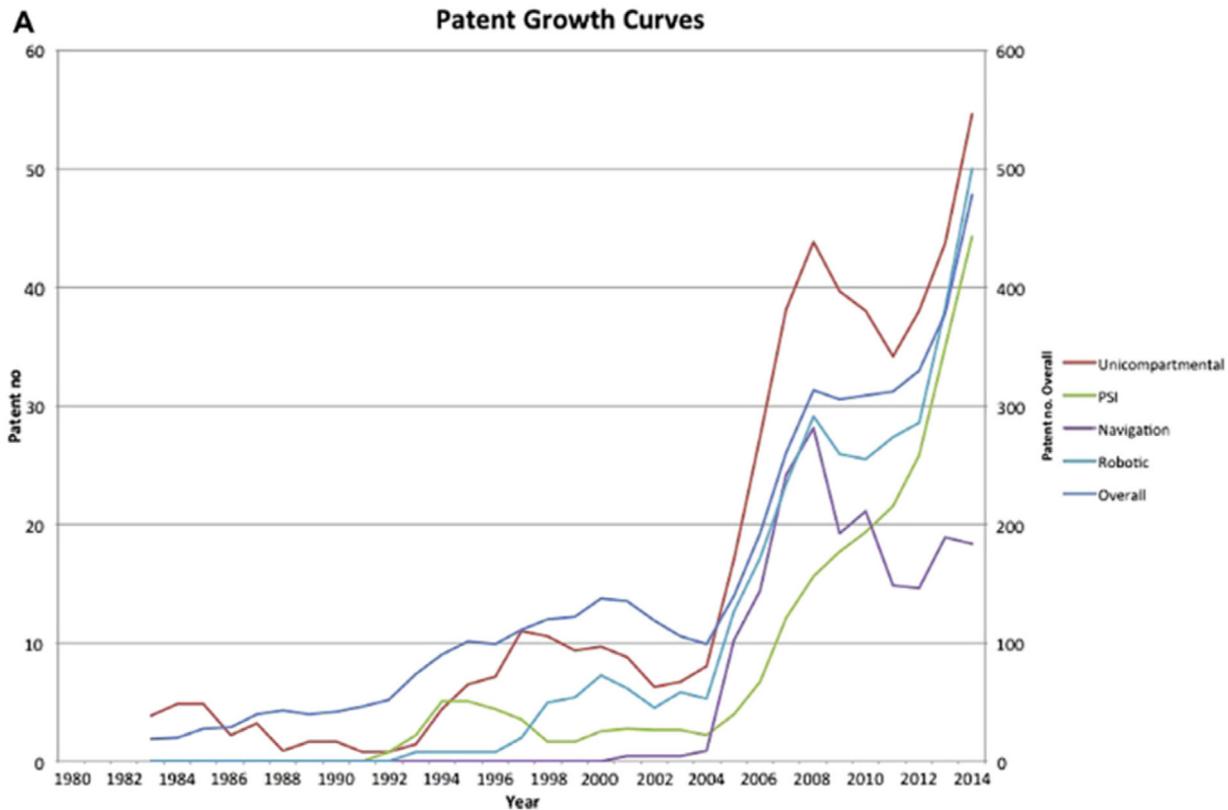


Figure 2. Graph of the normalized patent growth curve of the individual technology clusters (left hand axis) and the overall knee arthroplasty patent curve (right hand axis). Reprinted from The Journal of Arthroplasty, Vol 31/6, David M. Dalton, Thomas P. Burke, Enda G. Kelly, Paul D. Curtin, Quantitative Analysis of Technological Innovation in Knee Arthroplasty Using Patent and Publication Metrics to Identify Developments and Trends, 1366–1372. Copyright (2016), with permission from Elsevier.

came “semi-active robotic technology”, “controlled-forced robotic technology” or “haptic controlled technology” in which the surgeon was in charge in controlling a handheld device. Acrobot® (Acrobot Company Ltd, London, U.K.) was the first of this generation and was used for UKA surgery [33].

Paradoxically, navigation technology in orthopaedics came after robotics was introduced. The first CT-based navigation system was developed and used in 1994 in Pittsburgh by DiGioia and his team, who performed a computer-assisted guided hip cup replacement [34]. Other teams from all over the world worked on similar image-based navigation systems, such as in Japan for image guided hip replacement [35], in Switzerland for peri-acetabular reconstructions [36] or in the UK for femoral neck fractures [37].

Image-free or CT-free navigation, also called “surgeon-defined anatomy” technology, came in the early nineties with ACL reconstruction [38]. The first computer-assisted total knee replacement (TKR) system, based on similar concepts, was performed in 1997 [39,40,41]. In the same year, individual templates, also named patient specific instrumentation (PSI) or patient-specific-jigs, were introduced by Radermacher and later revived by Hafez [42,43].

More recently there has been an increase in the number of robotic orthopaedic technologies, with one of the front runners being MAKO® (Mako Surgical Corp., Florida, U.S.) [44], but many others have followed, such as ROSA® (Medtech, Montpellier, France) [45] and NavioPFS systems (Blue Belt Technologies, S&N, Pittsburgh, U.S.) [46]. These robots are all “hand-controlled semi-active robots”; the MAKO® and ROSA® using image technology but the NavioPFS® using only intra-operative anatomical and kinematic data. More recently, lightweight concepts such as the

Mazor® (Mazor Robotics, Caesarea, Israel), used for minimally invasive spinal surgery [47], and the OMNIBotics™ (Omnirobotic, Massachusetts, U.S.) [48] system used for total knee replacements have arisen.

6. Impact of CAOS on general “orthopaedic forum”

In June 2016, Dalton et al. published a very relevant article we would like to refer to as the common theme of this section [57]. Between 1980 and 2014, the authors examined patents and papers in relation to knee surgery and sorted them into four clusters of innovations, which could be used to link patents and publications: Unicompartmental Knee Replacement (UKR), Patient Specific Instrumentation (PSI), Navigation and Robotics. Three of these are part of the CAOS technology “family”. The patents in each cluster are shown in Figure 2. Since 2004, the ratio between patents and publications increased from approximately 1:10 in 2004 to almost 1:3 in 2014 showing industry-driven innovation on technology introduction in the field of knee arthroplasty (Fig. 3).

We investigated, along this chapter, the role of the industry in the introduction of any disruptive technology using the above quoted paper as a guideline and we also explore what may have been the role of CAOS in challenging some conventional surgical concepts. For publications we reproduced and extended the Dalton figures to 2018 and added categories of alignment and balancing both with and without CAS. Using the same methodology as Dalton et al. with search terms in Pubmed were as Table 1 with date range set to 1980/01/01 to 2018/12/31. We also searched for papers on alignment with and without CAS (Table 1). Publication numbers were normalised to 2014 using the following formula as per

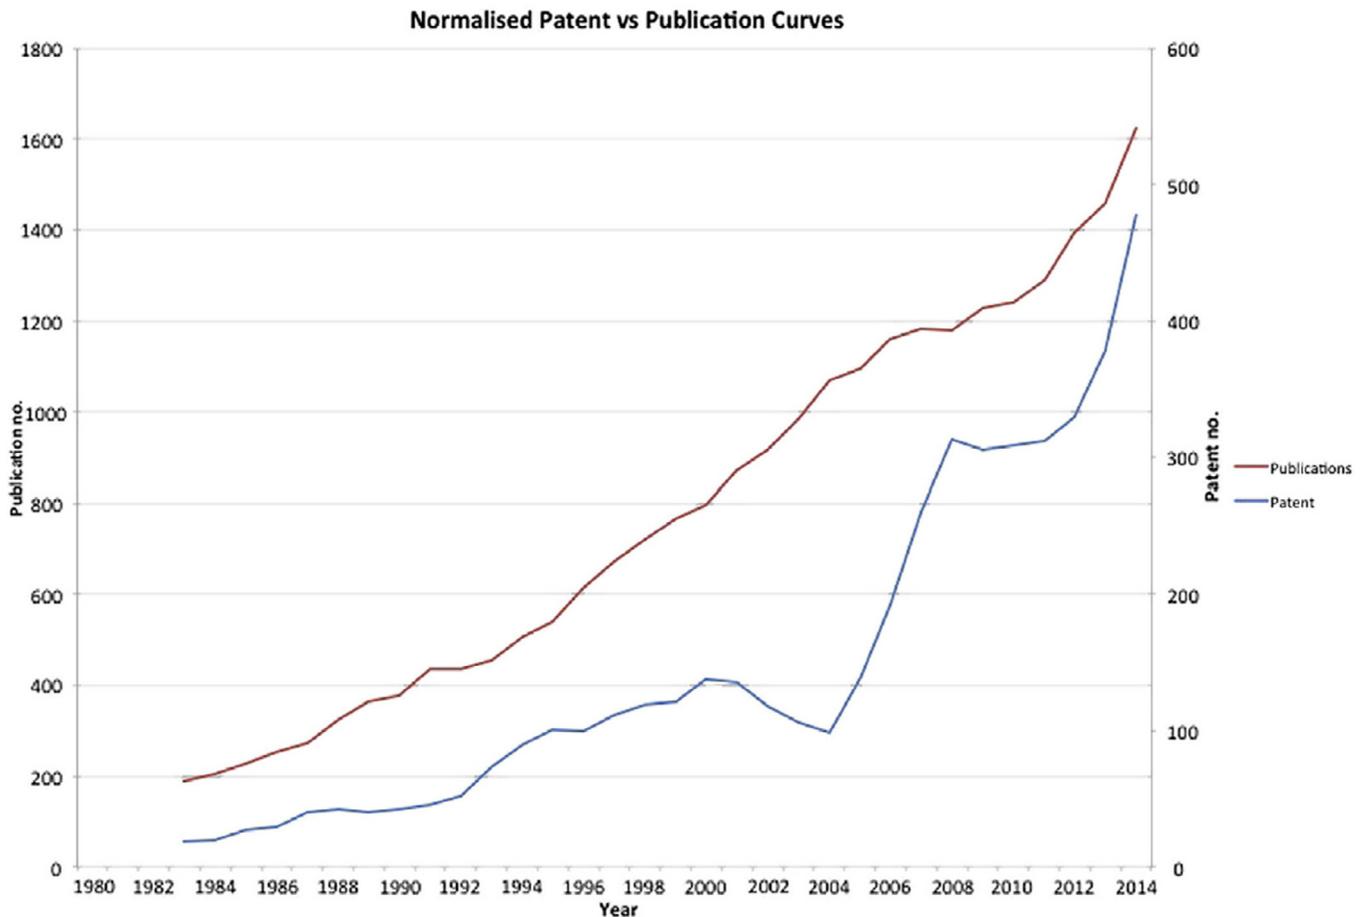


Figure 3. Graph of the overall normalised publication and patent curves again one another. Reprinted from The Journal of Arthroplasty, Vol 31/6, David M. Dalton, Thomas P. Burke, Enda G. Kelly, Paul D. Curtin, Quantitative Analysis of Technological Innovation in Knee Arthroplasty Using Patent and Publication Metrics to Identify Developments and Trends, 1366-1372, Copyright (2016), with permission from Elsevier.

Dalton et al.

$$II_i^{normalised} = \frac{II_i^{original}}{c_i}$$

$$where\ c_i = \frac{t_i}{t_{2014}}$$

where II is the innovation index (number of patents or publications in area), i is year, t is total number of patents granted or paper published and c is the innovation constant. Data were then plotted using a 4-period moving average as per Dalton et al. [57].

Between 2001 and 2004, the normalised number of publications regarding navigation multiplied by 10 (Fig. 4). At the time, most of the large global multinational orthopaedic companies had little expertise with CAOS systems apart from Stryker and Medtronic [8,58]. Most of the systems commercialised at the time were from smaller orthopaedic allied companies, e.g., Brainlab/München, Germany; Aesculap/ B Braun Tuttlingen Germany; OrthoSoft, Montreal, Canada [59].

Whether this sudden interest in CAOS made the larger companies react vigorously or not is difficult to confirm due to their strategic secrecy. However, it is clear that from 2003 onwards [60] a wave of publications, supported by the large corporations, promoted Minimally Invasive Surgery (MIS) for both hip and knee arthroplasty [61,62], which created a temporary diversion from the adoption of CAOS technology [63].

In 2014, we published a paper examining the reasons why CAOS was not mainstream at the time, as opposed to laparoscopic surgery and neuro-stereotactic guided surgery as both of them

Table 1

Technology group	Search terms
Unicondylar	("knee arthroplasty" OR "knee replacement") AND (unicondylar OR uni OR unicompartmental)
Patient specific implants	("knee arthroplasty" OR "knee replacement") AND (custom OR customized OR customised OR patient-specific OR personalized OR personalised)
Navigation	("knee arthroplasty" OR "knee replacement") AND navigation
Robotics	("knee arthroplasty" OR "knee replacement") AND (robot OR robotics OR robotic)
Alignment and balancing with CAS	("knee arthroplasty" OR "knee replacement") AND (alignment OR balance OR balancing OR soft-tissue OR "soft tissue") AND (navigation OR CAS OR "computer aided" OR "computer assisted" OR computer-aided OR computer-assisted OR robot OR robotics OR robotic)
Alignment and balancing without CAS	("knee arthroplasty" OR "knee replacement") AND (alignment OR balance OR balancing OR soft-tissue OR "soft tissue") NOT (navigation OR CAS OR "computer aided" OR "computer assisted" OR computer-aided OR computer-assisted OR robot OR robotics OR robotic)

are unchallenged methods in their field [59]. Many factors limited the spread of CAOS for wide adoption in total knee replacement (TKA), the object of our study, because of its perceived risks, additional surgical times and additional attendant costs [1]. Nonetheless, we found that two main factors limiting CAOS expansion were

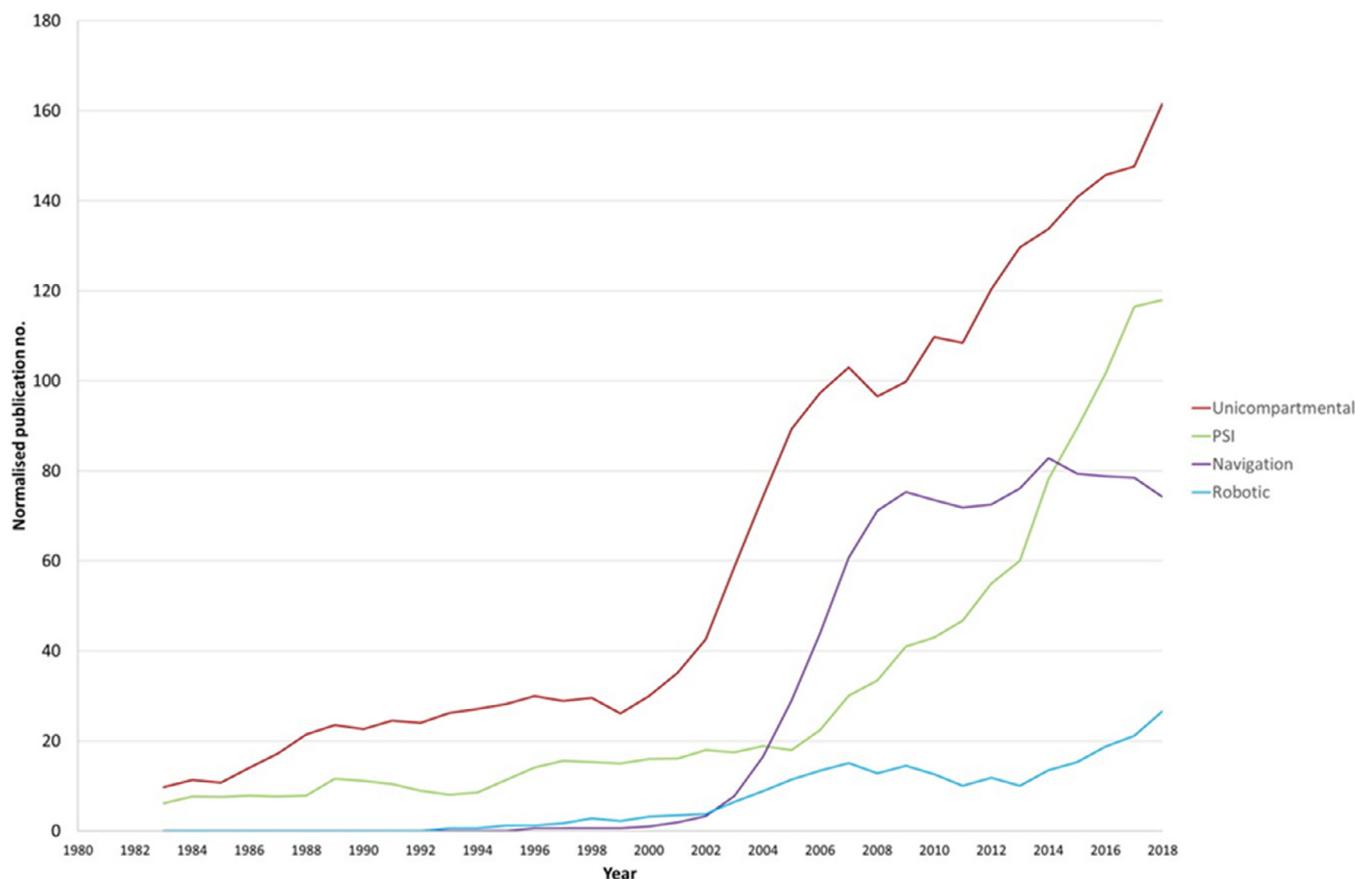


Figure 4. Normalised (to 2014) publication growth curves of the individual technology clusters of unicompartmental knee arthroplasty, PSI (patient specific instrumentation), navigation and robotics from 1980 to 2018.

ergonomics and economics [59]. Zheng et al. confirmed the first factor in his recent review and wrote “that one of the barriers to adoption of navigation” comes from “intra-operative glitches, unreliable accuracy, frustration with intra-operative registration and line of sight issues” [5].

According to Dalton et al. between 2004 and 2008, the number of patents registered under the “knee replacement” or “knee arthroplasty” label by industry grew steeply (Fig. 2). We could deduce from this, that the orthopaedic industry responded to the demand for CAOS and invested in new and better designed systems to match surgeons’ expectations. The number of publications rocketed during this period showing solid evidence of interest in the technology but also genuine vigilance from orthopaedic community in order to avoid worrying past experiences [64].

Ergonomic issues generated early scepticism in CAOS technology immediately after its introduction. Moreover, studies revealed fractures related to pin tracker fixation [65–67], infections on trackers sites [58,68] and lengthy surgery too [69]. Some early CAOS prototypes were probably launched too quickly, driven by the desire to be first, or the need to counteract competition. Without the correct support and training, these issues created fear in some of the early adopters [70]. However, later evidence did not confirm the initial impressions regarding the increase of complication rates but undoubtedly emphasised the increasing operative time due to the additional manipulations compared to conventional knee surgery [71].

Despite, in 2007, Novack concluding that CAOS navigation was potentially a cost-effective or cost-saving addition to TKA [73], economics was found to be one of the main issues limiting CAOS adoption, not only due to the high capital cost of the systems themselves, but also due to the overall overhead cost related to

increased length of surgery [72] and increased operating expenses with regards to inventory and surgical assistances [59].

The number of patents dedicated to navigation after 2008 reduced, whereas more investment was directed towards on PSI and two years later towards robotic technologies [57] (Fig. 2). Also by 2008, the number of publications for navigation declined whereas they increased for PSI [74,75]. It can be postulated, therefore, that the industry felt that investing more into PSI may, on the one hand, solve the ergonomic issues surgeons complained about but also, on the other hand, may solve their economic problems related to navigation.

The original claims for using CAOS, and specifically navigation, was that the technology would be more accurate and precise than conventional surgery, enhancing the three-dimensional position and alignment of joint replacements, spine screws or the safe bone/tissue resection in orthopaedic oncology [4]. While the evidence demonstrating the superiority of knee navigation over conventional instrumentation in accuracy and precision for alignment grew, some surgeons questioned the concept of alignment itself. It is difficult to identify what triggered this trend whether it is “safe vigilance reaction”, “backfire effect” or, “confirmation bias” amongst orthopaedic community and companies [71,76–78]. Dividing the number of papers published on knee alignment and TKA between 1976 and 2018 into those related to CAOS and those which are not, it seems clear to use that CAOS technology drove the discussion associated with knee replacement as far as alignment and balancing are concerned (Fig. 5). Therefore, challenging the concept of alignment was maybe a natural evolution to the discussion.

After challenging the evidence on accuracy and precision of CAOS systems in knee arthroplasty navigation, a dispute also arose

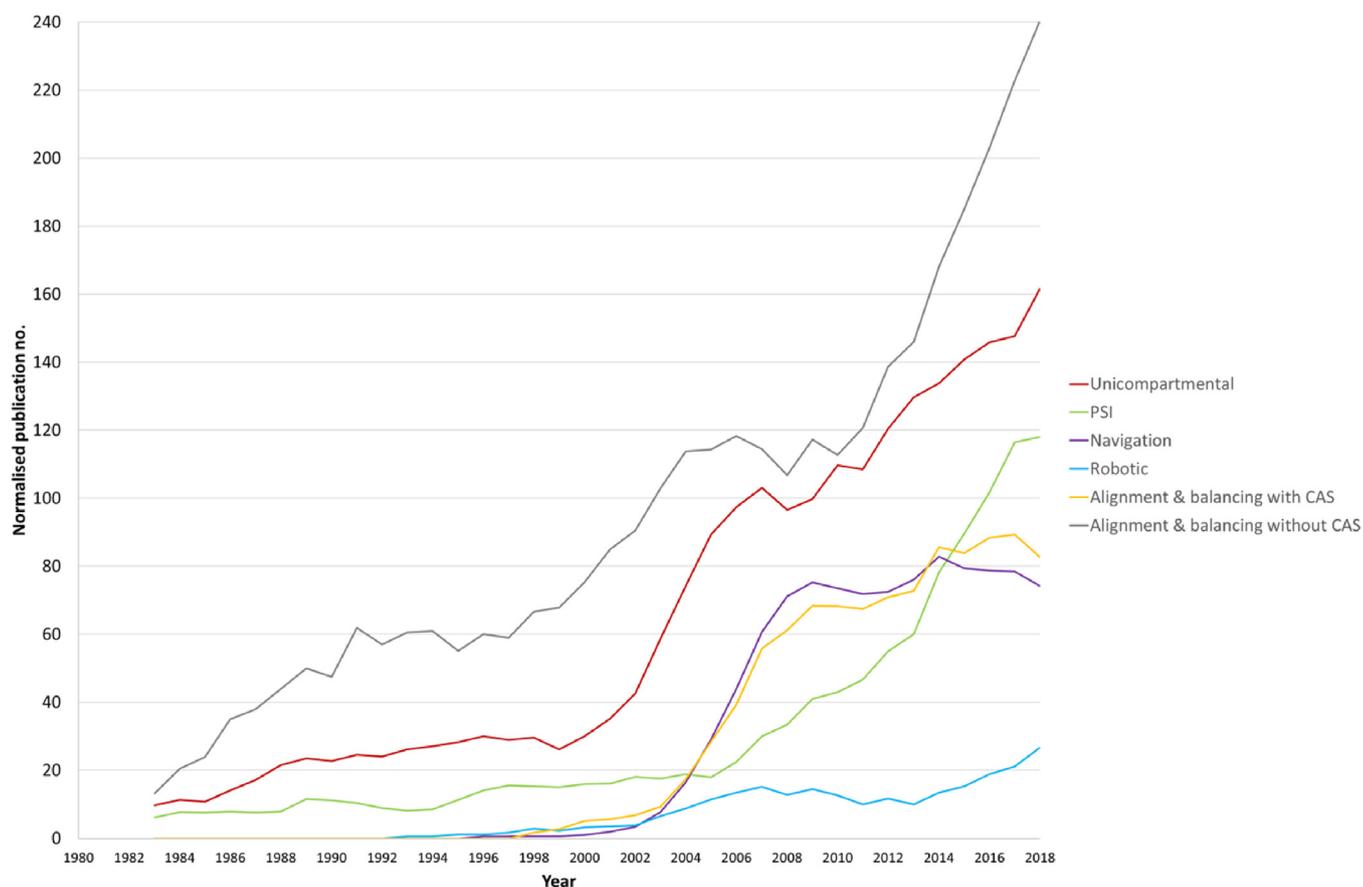


Figure 5. Relationship between alignment and balancing publications with CAS (yellow) and without (black). The steep increase in alignment without CAS (starting around 2010) follows the increase of papers with CAS (2002 to 2008).

around the lack of evidence of patient functional improvements [79–83]. Siston et al. [71] had already argued in 2007 the lack of evidence in any kinematic knee improvement after CAOS knee replacements. The combination of a lack of strong evidence of functional improvements and controversies around alignment in knee arthroplasty potentially fuelled new technological concepts, such as the so-called kinematic alignment, driven by PSI, more popular after 2014 according to number of publication (Figs. 4 and 5). This may have suggested that accuracy and precision in knee replacement may not be paramount as we thought [84,85].

In the same vein, some argued about the lack of improvement of long-term implant survivorship in well-aligned knee replacements with or without navigation [86,87]. However, De Steiger et al. showed from Australian registry data that in 44,573 computer assisted primary TKAs (14.1% of total) there was a reduction in the overall rate of revision in patients less than 65 years old [88]. At the same time, new publications confirmed functional improvements after CAOS TKA. Rebal et al. showed that navigated TKAs had a higher increase in Knee Society Score at 3-months follow-up and at 12 months follow-up compared to conventional knee replacement [89].

As already mentioned, after 2010, the orthopaedic industry had invested heavily in robotic-assisted technology [90] despite the unsuccessful past market introduction [91–93], and less in navigation certainly to offset implant price reduction and the lack of instalments for the costly surgical trays/instruments [93]. Selling at a very high price, robots became suddenly appealing to the industry but on the other hand, high capital costs remained an obvious and significant restraining factor of in the use of this technology

[95–97]. Investment grew more abruptly by 2012 onwards where industry tried to change the paradigm from computer aided technology to robotic aided technology [90]. The Mako[®] robot was one of the drivers of robotics in orthopaedics in reviving UKA market clearly noticeable on Dalton et al. figures with growing number of publications in UKA but also patents related to UKA [98] (Figs. 2 and 3).

Mako[®] attracted Stryker[®], one of the leading orthopaedic majors in the world leading to the acquisition of Mako[®] for \$1.6 billion between 2012 and 2013 by Stryker, launching the “robot wars” between competitors. Smith & Nephew bought the Navio[®]/BlueBelt Technology for \$275 million in 2016, Zimmer bought the ROSA[®] robotic system for at least \$132 million, and more recently Johnson & Johnson invested in a new robot named Orthotaxy[®] for an undisclosed amount.

After 2014, while the number of publications increased for PSI, navigation and robotic publication numbers went to opposite direction in favour of the later to the former. This would confirm our previous statement about the “robot-war” between companies (Figs. 4 and 5).

Swank M. et al. suggested that capital cost of robotic knee arthroplasty maybe recovered in as few as two years if 50, 70, and 90 cases were performed in the first three years [97]. Moschetti et al. carried out a Markov analysis on UKA and showed that above 94 UKAs a year, robotic UKA is cost-effective [96]. All these studies speculated on significant better functional outcomes [51,99] and the potential reduction in revision [95].

In surgical fields other than arthroplasty, the additional accuracy afforded by navigation enhances patient safety and facilitates

more complex surgery to be attempted. However, in joint replacement, the additional benefit of navigation resides purely in the accuracy and resulting alignment itself: the technology is being used to replicate conventional surgery, as opposed to opening up new surgical possibilities. Indeed, the MAKO[®] is now being used to perform THR – a highly successful conventional operation. Therefore, in essence, to have a wider adoption of CAOS in arthroplasty, surgeons must admit, individually and as a community, that their conventional arthroplasty surgery could be performed “better” with computer-assistance and with increased cost-effectiveness. Some surgeons hold this view, whilst others do not. This cognitive dissonance amongst many orthopaedic surgeons, which has made them sceptical about CAOS for some years, may generate a complex conundrum for the orthopaedic industry promoting robotic systems as more accurate and precise than navigation, since today’s robotic systems are only navigators with a robotic tool. To quote Cartiaux et al. “It is not yet possible to say unequivocally that improvements in the accuracy of the assisted surgical gestures substantially impact the outcomes of surgical procedures” [4]. However, there are surgeries in orthopaedics where the consensus is convincingly in favour of CAOS such as in oncology [100], spine applications [101] or complex cases in arthroplasty [102].

7. Future of CAOS

CAOS combines many sorts of technologies and each one of the components is evolving along its own path. For example, sensors used with devices like the “VERASENSE Knee System”, (Ortho sensors, Dania FL, USA.) are the result of sustainable technology coming from microelectronics [103,104]. There are today dozens of different sensors measuring pH, temperature, motion, speed, etc.... all becoming smaller, being more efficient and more accurate [105]. This is how these nanotechnology or small sensors are now even used in some experimental surgical implants, like knee replacements. [106,107] The sensor is only an example of one technology that evolved on its own all over the years for the benefit of current or future CAOS systems.

We can divide the future of CAOS into four main categories:-

- (1) Improvement of image-guided surgery;
- (2) Navigation systems and peri-operative assessment devices;
- (3) Robotics and simulation;
- (4) Artificial intelligence, algorithms and simulation

1- Image-guided surgery.

Zheng and Nolte [108] reported a potential evolution in their paper published in 2015 with regards to a 2-D/3-D image stitching principle involving intra-operative C-arms, which could be used in spine surgery or trauma for long bone fractures. Combining MRI [109], CT data sets mainly used in spine surgery, as well as in oncology, will certainly benefit from this new technology. Statistical shape modelling [15,110] has great potential and it is true that the concept can be used with image-free technology, fluoroscopic images or even ultrasound tracking technology [14]. There is great potential to use all of those in joint reconstruction and revision in particular, but also complex primary joint replacements with severe deformities of large bone defects making difficult for surgeons to plan such abnormal anatomy. Therefore, a statistical model renders a better virtual anatomy construct to build up the missing parts. The other potential progress should come from the use of combined technology, such as EOSTM (EOS Imaging, Paris, France), which reduces considerably the radiation dose during joint x-ray assessment [111].

Hybrid CAOS systems are already under development and are able to combine all these image-guided tools, which will allow

the surgeon to not only plan prior to surgery but also guide surgical intervention more accurately and, most importantly, more easily than today.

2- New generation of navigation systems and perioperative data measurements:

A number of smaller, smarter and easier to use systems exist, utilising tablets and small tracking devices, such as the BrainLab Dash[®], (Munich Germany) [112], the OrthoAlign (Orthoalign Inc, Ca, US) system [113] and the NaviSwiss (Naviswiss AG, Switzerland) intra-operative portable system [114], new CAOS systems using sensors such as accelerometers such as eLIBRA[®] (Zimmer Biomet Warsaw Indiana, US) [115], navigation-based technology using Infra-Red (IR) tracking (PhysioPilot[®] Surgi-concept Ltd, UK) for perioperative kinematic knee measurements [116], accelerometers (BPM Pathway[®] UK), Electronic goniometers (HALO, Halo Medical Devices, Australia), Ultrasound tracking system [117]. These devices generate huge amount of data potentially correlating perioperative to intraoperative measurements and will help to understand phenomena currently beyond our perception.

3- Robotic and simulation devices.

A new generation of robotic-assisted surgical tools will be able to use complex data to execute better planning. Today, robotic technology is just performing our current knowledge of conventional surgery. For instance, there are still controversies on what defines the best indications for UKA or what is the best alignment for TKA. It is thought that robotics can “reduce inventory, eliminate surgical trays, improve workflow and surgical efficiency and show net cost neutrality” [94]. Furthermore, as market-driven evolution has meant CAOS only replicates current surgical techniques, the potential exists for CAOS to inspire surgeon-led innovation to develop new types of surgery, not possible with conventional tooling. For example, implant design and CAOS systems have not been co-developed, losing the potential for smaller, bone-sparing prostheses. Ultimately, lesion-specific, biofabricated, mini-implants, replacing only the damaged tissue with new tissue, may be the final goal of arthroplasty surgery.

4- Artificial Intelligence, Algorithms and simulation.

The volume of collected data will increase considerably and will enable a new understanding of patterns in joint kinematics and certainly will give the new generation of navigation planning. CAOS is still at the stage of “measuring data” without really knowing what the best use of these data is. Artificial intelligence applied to big data analysis will draw clearer guideline pathways for professionals working in locomotor pathology and will provide surgical recommendations helping surgeons to perform more reproducibly and more accurately individual solutions for specific patients. Big data analyses combining peri- and intraoperative measurements of implant alignment/position, functional outcomes, satisfaction, long-term durability and so forth will shed light on the best course of action. Today we are still relying on crude information and data, even with the use of CAOS which may still explain some reticence against it.

8. Conclusion

Computer Assisted Orthopaedic Surgery is no longer new. Several systems have been available for more than 20 years. Current systems and particularly the navigation systems are implementing mature technology whereas new robotic systems are using more advanced equipment which still requires assessments especially for those more recently launched on the market.

The original premises of the technology to make any surgery more accurate, more precise and reproducible in any circumstances

aiming to improve patient's functional outcomes and long-term results have not been fully proven. Despite vast amounts of evidence supporting the use of the technology, CAOS is still not mainstream. There are many reasons behind this slow uptake amongst the orthopaedic community which combine safe vigilance of surgeons, lack of strong evidence for long term benefits, additional cost of systems not offset by any third parties and mostly industry driven recommendation of practices.

The industry is still looking for the best model to put into operation: computer assisted technology or robotic assisted technology as it is referred today either for semantic or marketing reasons. Technology will find its place in orthopaedics once the commercial model is stable and comprehended enough by all parties involved in patient care. It took many years for endoscopy and arthroscopy in orthopaedics to become an undisputed technology in the field. In the later years, industry, health providers, practitioners and patients all claimed superiority of the pros with respect to the cons of this technology in routine practice. This has not happened in the field of CAOS yet.

According to BCC Research, the global surgical robotics and computer-assisted surgery market reached nearly \$3.5 billion in 2015 [118]. This market is expected to increase from \$4.0 billion in 2016 to \$6.8 billion in 2021 at a compound annual growth rate (CAGR) of 11.3% for 2016–2021 [118]. Undoubtedly, CAOS will expand over the coming years even though patients and even clinicians will still need to find their way into true information circulating on the web [119] and relevant evidence.

Indeed, CAOS is a broad family covering any technology from preoperative computer aided planning, intraoperative robotic assistance to postoperative computer measurements and therefore it includes under its umbrella many different systems and technology which do not have the same qualities.

In this paper, we reviewed some of key features of the past of CAOS, looked at the current “state of the art” and imagine some of the future options for CAOS that readers will encounter in coming years. We hope that this review will help provide a clearer perspective on this rather cluttered subject.

Declaration of Competing Interest

BBraun Aesculap Consulting Agreements for Mr Baines, Mr Deep. Golden Jubilee National Hospital Orthopaedic Research department receives support from Zimmer, Stryker and BBraun.

Acknowledgments

Many thanks to Ludovic Picard for assistance in manuscript preparation.

Funding

None.

Ethical approval

Not required.

References

- Joskowicz L, Hazan EJ. Computer aided orthopaedic surgery: incremental shift or paradigm change? *Med Image Anal* 2016;33:84–90. doi:10.1016/j.media.2016.06.036.
- Diamandis PH. The world in 2025: 8 predictions for the next 10 years. SingularityHub 2015. <https://singularityhub.com/2015/05/11/the-world-in-2025-8-predictions-for-the-next-10-years/>.
- Moravec H. When will computer hardware match the human brain? *J Evol Technol* 1998;1:1–12.
- Cartiaux O, Jenny J-Y, Joskowicz L. Accuracy of computer-aided techniques in orthopaedic surgery: how can it be defined, measured experimentally, and analyzed from a clinical perspective? *J Bone Joint Surg Am* 2017;99:e39. doi:10.2106/JBJS.15.01347.
- Zheng G, Nolte LP. Computer-assisted orthopedic surgery: current state and future perspective. *Front Surg* 2015;2:66. doi:10.3389/fsurg.2015.00066.
- Digioia AM, Jaramaz B, Nikou C, Labarca RS, Moody JE, Colgan BD. Surgical navigation for total hip replacement with the use of hipnav. *Oper Tech Orthop* 2000;10:3–8. doi:10.1016/S1048-6666(00)80036-1.
- Sugano N, Takao M, Sakai T, Nishii T, Miki H. Does CT-based navigation improve the long-term survival in ceramic-on-ceramic THA? *Clin Orthop Relat Res* 2012;470:3054–9. doi:10.1007/s11999-012-2378-4.
- Foley KT, Simon DA, Rampersaud YR. Virtual fluoroscopy: computer-assisted fluoroscopic navigation. *Spine (Phila Pa 1976)* 2001;26:347–51.
- Picard F, Deep K, Jenny JY. Current state of the art in total knee arthroplasty computer navigation. *Knee Surg Sport Traumatol Arthrosc* 2016;24:3565–74. doi:10.1007/s00167-016-4337-1.
- Ellapparadja P, Mahajan V, Deakin AH, Deep K. Reproduction of hip offset and leg length in navigated total hip arthroplasty: how accurate are we? *J Arthroplast* 2015;30:1002–7. doi:10.1016/j.arth.2015.01.027.
- Picard F, Gregori A, Leitner F. *Computer assisted orthopaedics: the image free concept in total knee arthroplasty*. 1st Edition. Berlin, Germany: Pro Business; 2007.
- Székely G, Nolte L-P. Image guidance in orthopaedics and traumatology: a historical perspective. *Med Image Anal* 2016;33:79–83. doi:10.1016/j.media.2016.06.033.
- Docquier P-L, Paul L, Cartiaux O, Delloye C, Banse X. Computer-assisted resection and reconstruction of pelvic tumor sarcoma. *Sarcoma* 2010;2010:1–8. doi:10.1155/2010/125162.
- Chen TK, Abolmaesumi P, Pichora DR, Ellis RE. A system for ultrasound-guided computer-assisted orthopaedic surgery. *Comput Aided Surg* 2005;10:281–92. doi:10.3109/10929080500390017.
- Fleute M, Lavallée S, Julliard R. Incorporating a statistically based shape model into a system for computer-assisted anterior cruciate ligament surgery. *Med Image Anal* 1999;3:209–22. doi:10.1016/S1361-8415(99)80020-6.
- Sugano N. Computer-assisted orthopedic surgery. *J Orthop Sci* 2003;8:442–8. doi:10.1007/s10776-002-0623-6.
- Jakopec M, Rodriguez Baena F, Harris SJ, Gomes P, Cobb J, Davies BL. The hands-on orthopaedic robot “acrobot”: early clinical trials of total knee replacement surgery. *IEEE Trans Robot Autom* 2003;19:902–11. doi:10.1109/TRA.2003.817510.
- Stindel E, Briard JL, Merloz P, Plaweski S, Dubrana F, Lefevre C, et al. Bone morphing: 3D morphological data for total knee arthroplasty. *Comput Aided Surg* 2002;7:156–68. doi:10.1002/igs.10042.
- Gruetzner P, Waelti H, Vock B, Hebecker A, Nolte L-P, Wentzensen A. Navigation using fluoro-CT technology. *Eur J Trauma* 2004;30:161–70. doi:10.1007/s00068-004-1328-6.
- Clarke RH, Horsley V. THE CLASSIC: on a method of investigating the deep ganglia and tracts of the central nervous system (cerebellum). *Br med J* 1906;1799-1800. *Clin Orthop Relat Res* 2007;463:3–6. doi:10.1097/BLO.0b013e31814d4d99.
- Spiegel EA, Wycis HT, Marks M, Lee AJ. Stereotaxic apparatus for operations on the human brain. *Science (80-)* 1947;106:349–50. doi:10.1126/science.106.2754.349.
- Kwoh YS, Hou J, Jonckheere EA, Hayati S. A robot with improved absolute positioning accuracy for ct guided stereotactic brain surgery. *IEEE Trans Biomed Eng* 1988;35:153–60. doi:10.1109/10.1354.
- Benabid AL, Cinquin P, Lavalle S, Le Bas JF, Demongeot J, de Rougemont J. Computer-driven robot for stereotactic surgery connected to CT scan and magnetic resonance imaging. *technological design and preliminary results. Appl Neurophysiol* 1987;50:153–4.
- McBeth PB, Louw DF, Rizun PR, Sutherland GR. Robotics in neurosurgery. *Am J Surg* 2004;188:68–75. doi:10.1016/j.amjsurg.2004.08.004.
- Schlöndorff G. Computer-assisted surgery: historical remarks. *Comput Aid Surg* 1998;3:150–2. doi:10.3109/10929089809148137.
- Bettega G, Payan Y, Mollard B, Boyer A, Raphaël B, Lavallée S. A simulator for maxillofacial surgery integrating 3D cephalometry and orthodontia. *Comput Aided Surg* 2000;5:156–65. doi:10.3109/10929080009148886.
- Hounsfield GN. Computerized transverse axial scanning (tomography): part 1. description of system. *Br J Radiol* 1973;46:1016–22. doi:10.1259/0007-1285-46-552-1016.
- Lauterbur PC. Image formation by induced local interactions: examples employing nuclear magnetic resonance. *Nature* 1973;242:190–1. doi:10.1038/242190a0.
- Lorensen WE, Cline HE. Marching cubes: a high resolution 3D surface construction algorithm. In: *Proceedings of the 14th annual conference on computer graphics and interactive techniques-SIGGRAPH '87*. ACM Press; 1987. p. 163–9. doi:10.1145/37401.37422.
- Aldinger G, Fischer A, Kurtz B. Computer-aided manufacture of individual endoprostheses. *Arch Orthop Trauma Surg* 1983;102:31–5. doi:10.1007/BF00443036.
- Hennessey D, Anderson M, Lozano-Calderón S. Complex pelvic reconstruction using patient-specific instrumentation and a 3D-Printed custom implant following tumor resection. *J Hip Surg* 2018;02:061–7. doi:10.1055/s-0037-1618581.
- Taylor RH, Mittelstadt BD, Paul HA, Hanson W, Kazanzides P, Zuhars JF, et al. An image-directed robotic system for precise orthopaedic surgery. *IEEE Trans Robot Autom* 1994;10:261–75. doi:10.1109/70.294202.
- Davies BL, Harris SJ, Lin WJ, Hibberd RD, Middleton R, Cobb JC. Active compliance in robotic surgery—the use of force control as a dynamic

- constraint. *Proc Inst Mech Eng Part H J Eng Med* 1997;211:285–92. doi:10.1243/0954411971534403.
- [34] Digiioia AM, Simon D, Jaramaz B, Blackwell M, Morgan FM, O'Toole RV, et al. HipNav: pre-operative planning and intra-operative navigational guidance for acetabular implant placement in total hip replacement surgery. In: *Proceedings of the computer assisted orthopaedic surgery symposium Bern Switzerland*; 1995.
- [35] Sato Y, Sasama T, Sugano N, Nakahodo K, Nishii T, Ozono K, et al. Intraoperative simulation and planning using a combined acetabular and femoral (CAF) navigation system for total hip replacement. In: *Proceedings of the international conference on medical image computing and computer-assisted intervention*. Springer; 2000. p. 1114–25. doi:10.1007/978-3-540-40899-4_116.
- [36] Langlotz F, Stucki M, Bächler R, Scheer C, Ganz R, Berlemann U, et al. The first twelve cases of computer assisted periacetabular osteotomy. *Comput Aided Surg* 1997;2:317–26. doi:10.3109/10929089709149831.
- [37] Viant WJ, Phillips R, Griffiths JG, Ozanian TO, Mohsen AMMA, Cain TJ, et al. A computer assisted orthopaedic surgical system for distal locking of intramedullary nails. *Proc Inst Mech Eng Part H J Eng Med* 1997;211:293–300. doi:10.1243/0954411971534412.
- [38] Dessenne V, Lavallée S, Julliard R, Orti R, Martelli S, Cinquin P. Computer-assisted knee anterior cruciate ligament reconstruction: first clinical tests. *J Image Guid Surg* 1995;1:59–64. 10.1002/(SICI)1522-712X(1995)1:1<59::AID-IGS9>3.0.CO;2-L.
- [39] Picard F, Leitner E, Raoult O, Saragaglia D. Computer assisted total knee arthroplasty. *rechn. verfahren orthopädie und unfallchirurgie*. Heidelberg: Steinkopff; 1999. p. 461–71. doi:10.1007/978-3-642-58699-6_29.
- [40] Leitner F, Picard F, Minfeldt R, Schulz JH, Cinquin P, Saragaglia D. *Computer assisted total knee arthroplasty*. MRCAS'97. Springer Verlag; 1997. p. 629–38.
- [41] Delp SL, Stulberg SD, Davies B, Picard F, Leitner F. Computer assisted knee replacement. *Clin Orthop Relat Res* 1998;354:49–56.
- [42] Radermacher K, Porthelme F, Anton M, Zimolung A, Kaspers G, Rau G, et al. Computer assisted orthopaedic surgery with image based individual templates. *Clin Orthop Relat Res* 1998;354:28–38.
- [43] Hafez MA, Chelule KL, Seedhom BB, Sherman KP. Computer-assisted total knee arthroplasty using patient-specific templating. *Clin Orthop Relat Res* 2006;443:184–92. doi:10.1097/01.blo.0000201148.06454.e4.
- [44] Roche M, O'Loughlin PF, Kendoff D, Musahl V, Pearle AD. Robotic arm-assisted unicompartmental knee arthroplasty: preoperative planning and surgical technique. *Am J Orthop (Belle Mead NJ)* 2009;38:10–15.
- [45] Chenin L, Peltier J, Lefranc M. Minimally invasive transformal lumbar interbody fusion with the ROSA™ spine robot and intraoperative flat-panel CT guidance. *Acta Neurochir (Wien)* 2016;158:1125–8. doi:10.1007/s00701-016-2799-z.
- [46] Lonner JH, Smith JR, Picard F, Hamlin B, Rowe PJ, Riches PE. High degree of accuracy of a novel image-free handheld robot for unicondylar knee arthroplasty in a cadaveric study. *Clin Orthop Relat Res* 2015;473:206–12. doi:10.1007/s11999-014-3764-x.
- [47] Shoham M, Burman M, Zehavi E, Joskowicz L, Batkilen E, Kunicher Y. Bone-mounted miniature robot for surgical procedures: concept and clinical applications. *IEEE Trans Robot Autom* 2003;19:893–901. doi:10.1109/TRA.2003.817075.
- [48] Plaskos C, Cinquin P, Lavallée S, Hodgson AJ. Praxiteles: a miniature bone-mounted robot for minimal access total knee arthroplasty. *Int J Med Robot Comput Assist Surg* 2005;1:67–79. doi:10.1002/rcs.59.
- [49] Sasaki H, Ishida K, Shibayama N, Takayama K, Hayashi S, Hashimoto S, et al. Comparison of coronal prosthetic alignment after total knee arthroplasty using 3 computer-assisted navigation systems. *Orthopedics* 2018;41:e621–8. doi:10.3928/01477447-20180711-02.
- [50] Song E-K, Seon J-K. *Robotic total knee arthroplasty*. *comput. assist. orthop. surg. hip knee*. Singapore: Springer Singapore; 2018. p. 27–40. doi:10.1007/978-981-10-5245-3_3.
- [51] Gilmour A, MacLean AD, Rowe PJ, Banger MS, Donnelly I, Jones BG, et al. Robotic-Arm-Assisted vs conventional unicompartmental knee arthroplasty. The 2-Year clinical outcomes of a randomized controlled trial. *J Arthroplast* 2018;33:S109–15. doi:10.1016/j.arth.2018.02.050.
- [52] Saragaglia D, Sigwalt L, Refaie R, Rubens-Duval B, Lateur G, Pailhé R. Influence of the post-operative axis on the clinical results of total knee replacement for severe varus deformities: does a slight residual varus improve the results? *Int Orthop* 2018;1–6. doi:10.1007/s00264-018-4092-7.
- [53] Hüfner T, Kfuri M, Galanski M, Bastian L, Loss M, Pohlmann T, et al. New indications for computer-assisted surgery: tumor resection in the pelvis. *Clin Orthop Relat Res* 2004;426:219–25. doi:10.1097/01.blo.0000138958.11939.94.
- [54] Farfalli GL, Albergo JJ, Ritacco LE, Ayerza MA, Milano FE, Aponte-Tinao LA. What is the expected learning curve in computer-assisted navigation for bone tumor resection? *Clin Orthop Relat Res* 2017;475:668–75. doi:10.1007/s11999-016-4761-z.
- [55] Rampersaud YR, Lee K-S. Fluoroscopic computer-assisted pedicle screw placement through a mature fusion mass. *Spine (Phila Pa 1976)* 2007;32:217–22. doi:10.1097/01.brs.0000251751.51936.3f.
- [56] Lonner JH, Moretti VM. The evolution of image-free robotic assistance in unicompartmental knee arthroplasty. *Am J Orthop (Belle Mead NJ)* 2016;45:249–54.
- [57] Dalton DM, Burke TP, Kelly EG., Curtin PD. Quantitative analysis of technological innovation in knee arthroplasty. *J Arthroplast* 2016;31:1366–72. doi:10.1016/j.arth.2015.12.031.
- [58] Krackow KA, Phillips MJ, Bayers-Thering M, Serpe L, Mihalko WM. Computer-assisted total knee arthroplasty: navigation in TKA. *Orthopedics* 2003;26:1017–23.
- [59] Picard F, Clarke J, Gregori A, Deep K. Computer assisted knee replacement surgery: is the movement mainstream? *Orthop Musc Syst* 2014;03. doi:10.4172/2161-0533.1000153.
- [60] Picard F, Deakin A, Balasubramanian N, Gregori A. Minimally invasive total knee replacement: techniques and results. *Eur J Orthop Surg Traumatol* 2018;28:781–91. doi:10.1007/s00590-018-2164-4.
- [61] Berry DJ, Berger RA, Callaghan JJ, Dorr LD, Duwelius PJ, Hartzband MA, et al. Symposium: minimally invasive total hip arthroplasty. *JBJS* 2003;85:2235–46.
- [62] Laskin RS, Bekas B, Phongjunakorn A, Pittors K, Davis J, Shim J-C, et al. Minimally invasive total knee replacement through a mini-midvastus incision. *Clin Orthop Relat Res* 2004;428:74–81. doi:10.1097/01.blo.0000148582.86102.47.
- [63] Lüring C, Beckmann J, Haiböck P, Perlick L, Grifka J, Tingart M. Minimal invasive and computer assisted total knee replacement compared with the conventional technique: a prospective, randomised trial. *Knee Surg Sport Traumatol Arthrosc* 2008;16:928–34. doi:10.1007/s00167-008-0582-2.
- [64] Langton DJ, Jameson SS, Joyce TJ, Hallab NJ, Natsu S, Nargol AVF. Early failure of metal-on-metal bearings in hip resurfacing and large-diameter total hip replacement. *J Bone Joint Surg Br* 2010;92-B:38–46. doi:10.1302/0301-620X.92B1.22770.
- [65] Wysocki RW, Sheinkop MB, Virkus WW, Della Valle CJ. Femoral fracture through a previous pin site after computer-assisted total knee arthroplasty. *J Arthroplast* 2008;23:462–5. doi:10.1016/j.arth.2007.03.019.
- [66] Ossendorf C, Fuchs B, Koch P. Femoral stress fracture after computer navigated total knee arthroplasty. *Knee* 2006;13:397–9. doi:10.1016/j.knee.2006.06.002.
- [67] Seon JK, Song EK, Yoon TR, Seo HY, Cho SG. Tibial plateau stress fracture after unicondylar knee arthroplasty using a navigation system: two case reports. *Knee Surg Sport Traumatol Arthrosc* 2007;15:67–70. doi:10.1007/s00167-006-0097-7.
- [68] Sparmann M, Wolke B, Czupalla H, Banzer D, Zink A. Positioning of total knee arthroplasty with and without navigation support: a prospective, randomised study. *J Bone Joint Surg Br* 2003;85:830–5.
- [69] Friederich N, Verdonk R. The use of computer-assisted orthopedic surgery for total knee replacement in daily practice: a survey among ESSKA/SGO-SSO members. *Knee Surg Sport Traumatol Arthrosc* 2008;16:536–43. doi:10.1007/s00167-008-0518-x.
- [70] Bellemans J, Vandenuecker H, Vanlauwe J. Robot-assisted total knee arthroplasty. *Clin Orthop Relat Res* 2007;464:111–16. doi:10.1097/BLO.0b013e318126c0c0.
- [71] Siston RA, Giori NJ, Goodman SB, Delp SL. Surgical navigation for total knee arthroplasty: a perspective. *J Biomech* 2007;40:728–35. doi:10.1016/j.jbiomech.2007.01.006.
- [72] Bähthi H, Perlick L, Tingart M, Lüring C, Zurakowski D, Grifka J. Alignment in total knee arthroplasty. a comparison of computer-assisted surgery with the conventional technique. *J Bone Joint Surg Br* 2004;86:682–7.
- [73] Novak EJ, Silverstein MD, Bozic KJ. The cost-effectiveness of computer-assisted navigation in total knee arthroplasty. *J Bone Joint Surg Am* 2007;89:2389–97. doi:10.2106/JBJS.F.01109.
- [74] Hafez MA, Chelule KL, Seedhom BB, Sherman KP. Computer-assisted total knee arthroplasty using patient-specific templating. *Clin Orthop Relat Res* 2006;443:184–92. doi:10.1097/01.blo.0000201148.06454.e4.
- [75] Lombardi AV, Berend KR, Adams JB. Patient-specific approach in total knee arthroplasty. *Orthopedics* 2008;31:927–30.
- [76] Mason JB, Fehring TK, Estok R, Banel D, Fahrback K. Meta-Analysis of alignment outcomes in computer-assisted total knee arthroplasty surgery. *J Arthroplast* 2007;22:1097–106. doi:10.1016/j.arth.2007.08.001.
- [77] Parratte S, Pagnano MW, Trousdale RT, Berry DJ. Effect of postoperative mechanical axis alignment on the fifteen-year survival of modern, cemented total knee replacements. *J Bone Jt Surg Am Vol* 2010;92:2143–9. doi:10.2106/JBJS.I.01398.
- [78] Bellemans J, Colyn W, Vandenuecker H, Victor J. The Chitranjan Ranawat award: is neutral mechanical alignment normal for all patients? The concept of constitutional varus. *Clin Orthop Relat Res* 2012;470:45–53. doi:10.1007/s11999-011-1936-5.
- [79] Kinzl L, Gebhard F, Keppler P. Total knee arthroplasty—navigation as the standard. *Der Chir* 2004;75:976–81. doi:10.1007/s00104-004-0943-4.
- [80] Hofmann AA. Computer-assisted surgery for total knee arthroplasty: more than just “boy toys” for the passionate few. *Point Orthop* 2005;28:940–942.
- [81] Hungerford DS. Computer-assisted surgery: still just “boy toys” for the passionate few. *Counterpoint Orthop* 2005;28:941.
- [82] Choong PF, Dowsey MM, Stoney JD. Does accurate anatomical alignment result in better function and quality of life? Comparing conventional and computer-assisted total knee arthroplasty. *J Arthroplast* 2009;24:560–9. doi:10.1016/j.arth.2008.02.018.
- [83] Matsumoto T, Nakano N, Lawrence JE, Khanduja V. Current concepts and future perspectives in computer-assisted navigated total knee replacement. *Int Orthop* 2018. doi:10.1007/s00264-018-3950-7.
- [84] Howell SM, Hull ML. *Kinematic alignment in total knee arthroplasty*. Insall & Scott surgery of the knee. 5th ed. Philadelphia, PA, USA: Elsevier, Churchill Livingstone; 2012. p. 1255–68.

- [85] Howell SM, Hodapp EE, Vernace JV, Hull ML, Meade TD. Are undesirable contact kinematics minimized after kinematically aligned total knee arthroplasty? An intersurgeon analysis of consecutive patients. *Knee Surg Sport Traumatol Arthrosc* 2013;21:2281–7. doi:10.1007/s00167-012-2220-2.
- [86] Kim Y-H, Park J-W, Kim J-S. 2017 Chitranjan S. Ranawat award. *Clin Orthop Relat Res* 2018;476:6–15. doi:10.1007/s11999-0000000000000000.
- [87] Schemitsch EH. In younger patients with end-stage knee osteoarthritis, computer-assisted versus conventional total knee arthroplasty did not improve function at 15 years. *J Bone Jt Surg* 2018;100:1982. doi:10.2106/JBJS.18.00917.
- [88] de Steiger RN, Liu Y-L, Graves SE. Computer navigation for total knee arthroplasty reduces revision rate for patients less than sixty-five years of age. *J Bone Jt Surg-Am Vol* 2015;97:635–42. doi:10.2106/JBJS.M.01496.
- [89] Rebal BA, Babatunde OM, Lee JH, Geller JA, Patrick DA, Macaulay W. Imageless computer navigation in total knee arthroplasty provides superior short term functional outcomes: a meta-analysis. *J Arthroplast* 2014;29:938–44. doi:10.1016/j.arth.2013.09.018.
- [90] Cortez MF. Stryker to buy mako for \$1.65 billion for robotic surgery. Bloomberg 2013. <https://www.bloomberg.com/news/articles/2013-09-25/stryker-to-buy-mako-for-1-65-billion-for-robotic-surgery-1->
- [91] Siebert W, Mai S, Kober R, Heeck PF. Technique and first clinical results of robot-assisted total knee replacement. *Knee* 2002;9:173–80. doi:10.1016/S0968-0160(02)00015-7.
- [92] Jakopc M, Harris SJ, Rodriguez y Baena F, Gomes P, Cobb J, Davies BL. The first clinical application of a “hands-on” robotic knee surgery system. *Comput Aid Surg* 2001;6:329–39. doi:10.1002/igs.10023.
- [93] Park SE, Lee CT. Comparison of robotic-assisted and conventional manual implantation of a primary total knee arthroplasty. *J Arthroplast* 2007;22:1054–9. doi:10.1016/j.arth.2007.05.036.
- [94] Lonner JH, Fillingham YA. Pros and cons: a balanced view of robotics in knee arthroplasty. *J Arthroplast* 2018;33:2007–13. doi:10.1016/j.arth.2018.03.056.
- [95] Lonner JH. Robotically assisted unicompartmental knee arthroplasty with a handheld image-free sculpting tool. *Orthop Clin North Am* 2016;47:29–40. doi:10.1016/j.jocl.2015.08.024.
- [96] Moschetti WE, Konopka JF, Rubash HE, Genuario JW. Can robot-assisted unicompartmental knee arthroplasty be cost-effective? a Markov decision analysis. *J Arthroplast* 2016;31:759–65. doi:10.1016/j.arth.2015.10.018.
- [97] Swank ML, Alkire M, Condit M, Lonner JH. Technology and cost-effectiveness in knee arthroplasty: computer navigation and robotics. *Am J Orthop (Belle Mead NJ)* 2009;38:32–6.
- [98] Pearle AD, O’Loughlin PF, Kendoff DO. Robot-assisted unicompartmental knee arthroplasty. *J Arthroplast* 2010;25:230–7. doi:10.1016/j.arth.2008.09.024.
- [99] Bell SW, Anthony I, Jones B, MacLean A, Rowe P, Blyth M. Improved accuracy of component positioning with robotic-assisted unicompartmental knee arthroplasty. *J Bone Jt Surg* 2016;98:627–35. doi:10.2106/JBJS.15.00664.
- [100] Wong K-C, Niu X, Xu H, Li Y, Kumta S. Computer navigation in orthopaedic tumour surgery. *Adv. Exp. Med. Biol.* 2018;1093:315–26. doi:10.1007/978-981-13-1396-7_24.
- [101] Tian W, Zeng C, An Y, Wang C, Liu Y, Li J. Accuracy and postoperative assessment of pedicle screw placement during scoliosis surgery with computer-assisted navigation: a meta-analysis. *Int J Med Robot Comput Assist Surg* 2017;13:e1732. doi:10.1002/rcs.1732.
- [102] Chou W-Y, Ko J-Y, Wang C-J, Wang F-S, Wu R-W, Wong T. Navigation-Assisted total knee arthroplasty for a knee with malunion of the distal femur. *J Arthroplast* 2008;23:1239.e13–1239.e17. doi:10.1016/j.arth.2007.11.001.
- [103] Gustke K. Use of smart trials for soft-tissue balancing in total knee replacement surgery. *J Bone Joint Surg Br* 2012;94:147–50. doi:10.1302/0301-620X.94B11.30621.
- [104] Gustke KA, Golladay GJ, Roche MW, Elson LC, Anderson CR. A new method for defining balance: promising short-term clinical outcomes of sensor-guided tka. *J Arthroplast* 2014;29:955–60. doi:10.1016/j.arth.2013.10.020.
- [105] Bansal AK, Hou S, Kulyk O, Bowman EM, Samuel IDW. Wearable organic optoelectronic sensors for medicine. *Adv Mater* 2015;27:7638–44. doi:10.1002/adma.201403560.
- [106] Nielsen ES, Hsu A, Patil S, Colwell CW, D’Lima DD. Second-Generation electronic ligament balancing for knee arthroplasty: a cadaver study. *J Arthroplast* 2018;33:2293–300. doi:10.1016/j.arth.2018.02.057.
- [107] Mentink MJA, Van Duren BH, Murray DW, Gill HS. A novel flexible capacitive load sensor for use in a mobile unicompartmental knee replacement bearing: an in vitro proof of concept study. *Med Eng Phys* 2017;46:44–53. doi:10.1016/j.medengphy.2017.05.002.
- [108] Chen C, Kojcev R, Haschtmann D, Fekete T, Nolte L, Zheng G. Ruler based automatic C-Arm image stitching without overlapping constraint. *J Digit Imaging* 2015;28:474–80. doi:10.1007/s10278-014-9763-3.
- [109] Wong KC, Kumta SM, Antonio GE, Tse LF. Image fusion for computer-assisted bone tumor surgery. *Clin Orthop Relat Res* 2008;466:2533–41. doi:10.1007/s11999-008-0374-5.
- [110] Harris MD, Datar M, Whitaker RT, Jurrus ER, Peters CL, Anderson AE. Statistical shape modeling of cam femoroacetabular impingement. *J Orthop Res* 2013;31:1620–6. doi:10.1002/jor.22389.
- [111] Lazennec JY, Rousseau MA, Rangel A, Gorin M, Belicourt C, Brusson A, et al. Pelvis and total hip arthroplasty acetabular component orientations in sitting and standing positions: measurements reproducibility with EOS imaging system versus conventional radiographies. *Orthop Traumatol Surg Res* 2011;97:373–80. doi:10.1016/j.otsr.2011.02.006.
- [112] Balthis H. Brainlab dash®: iPod®-Based navigation system in total knee and hip replacements. *Computer and template assisted orthopedic surgery*. Berlin, Heidelberg: Springer Berlin Heidelberg; 2013. p. 89–95. doi:10.1007/978-3-642-29728-1_10.
- [113] Jones CW, Jerabek SA. Current role of computer navigation in total knee arthroplasty. *J Arthroplast* 2018;33:1989–93. doi:10.1016/j.arth.2018.01.027.
- [114] Widmer KH, Ottersbach A, Schroeder-Boersch H. Smart hand-held imageless navigation for augmented surgical quality and improved patient safety in total hip arthroplasty. *Orthop Proc* 2019;101:105. doi:10.1302/1358-992X.2019.5.105.
- [115] Fetto JF, Hadley S, Leffers KJ, Leslie CJ, Schwarzkopf R. Electronic measurement of soft-tissue balancing reduces lateral releases in total knee arthroplasty. *Bull NYU Hosp Jt Dis* 2011;69:285–8.
- [116] Alho R, Henderson F, Clarke J, Picard F, Deakin AH. Validation of a new and pre-validated set of non-invasive optical trackers used on the image-free physiopilot navigation system. *Abstr J Surg* 2015;23:S15eS134.
- [117] Washburn N, Onishi K, Wang JH-C. Ultrasound elastography and ultrasound tissue characterisation for tendon evaluation. *J Orthop Transl* 2018;15:9–20. doi:10.1016/j.jot.2018.06.003.
- [118] Kumar A. Medical robotics and computer-assisted surgery: The global market. BCC Research Market Research Report published May 2017.
- [119] Shemesh SS, Bronson MJ, Moucha CS. Computer-assisted total knee arthroplasty marketing and patient education: an evaluation of quality, content and accuracy of related websites. *Int Orthop* 2016;40:2003–9. doi:10.1007/s00264-016-3215-2.