

Clinical Study

# Value of standard radiographs, computed tomography, and magnetic resonance imaging of the lumbar spine in detection of intraoperatively confirmed pedicle screw loosening—a prospective clinical trial

José Miguel Spirig, MD<sup>a,\*</sup>, Reto Sutter, MD<sup>b</sup>, Tobias Götschi, MSc<sup>c</sup>,  
Nadja A. Farshad-Amacker, MD<sup>b</sup>, Mazda Farshad, Professor of Orthopaedics<sup>a</sup>

<sup>a</sup> Spine Division, University Hospital Balgrist, University of Zürich, Switzerland

<sup>b</sup> Department of Radiology, University Hospital Balgrist, University of Zürich, Switzerland

<sup>c</sup> Institute for Biomechanics, ETH Zürich, Switzerland

Received 19 February 2018; revised 18 June 2018; accepted 19 June 2018

## Abstract

**BACKGROUND CONTEXT:** Pedicle screw loosening is common after spinal fusion and can be associated with pseudoarthrosis and pain. With suspicion of screw loosening on standard radiographs, CT is currently considered the advanced imaging modality of choice. MRI with new metal artifact reduction techniques holds potential to be sensitive in detection of screw loosening. The sensitivity and specificity of either of the imaging modalities are yet clear.

**PURPOSE:** To evaluate the sensitivity and specificity of three different image modalities (standard radiographs, CT, and MRI) for detection of pedicle screw loosening.

**STUDY DESIGN/SETTING:** Cross-sectional diagnostic study.

**PATIENT SAMPLE:** Forty-one patients (159 pedicle screws) undergoing revision surgeries after lumbar spinal fusion between August 2014 and April 2017 with preoperative radiographs, CT, and MRI with spinal metal artifact reduction (STIR WARP and TSE high bandwidth sequences).

**OUTCOME MEASURES:** Sensitivity and specificity in detection of screw loosening for each imaging modality.

**METHODS:** Screw torque force was measured intraoperatively and compared with preoperative screw loosening signs such as peri-screw edema in MRI and peri-screw osteolysis in CT and radiographs. A torque force of less than 60 Ncm was used to define a screw as loosened.

**RESULTS:** Sensitivity and specificity in detection of screw loosening was 43.9% and 92.1% for MRI, 64.8% and 96.7% for CT, and 54.2% and 83.5% for standard radiographs, respectively.

**CONCLUSIONS:** Despite improvement of MRI with metal artifact reduction MRI technique, CT remains the modality of choice. Even so, CT fails to detect all loosened pedicle screws. © 2018 Elsevier Inc. All rights reserved.

## Keywords:

Metal artifact reduction; Radiolucent zone; Screw loosening; Spinal implant loosening; STIR; WARP

## Introduction

Pedicle screw fixation has become one of the standard methods of instrumentation for spinal fusion. The purpose of pedicle screw fixation is to increase the stability of the segments in order to increase the chance of bony fusion. One common complication is loosening of pedicle screws at the bone interface which, in the presence of pseudarthrosis, often result in revision surgery.

FDA device/drug status: Not applicable.

Author disclosure: **JMS:** Nothing to disclose. **RS:** Nothing to disclose.

**TG:** Nothing to disclose. **NAF:** Nothing to disclose. **MF:** Fellowship support: J&J (F)

\* Corresponding author. Spine Division, University Hospital Balgrist, University of Zürich, Switzerland. Tel.: +41 44 386 11 11.

E-mail addresses: [jose.spirig@balgrist.ch](mailto:jose.spirig@balgrist.ch), [jose.spirig@gmail.com](mailto:jose.spirig@gmail.com) (J.M. Spirig).

The frequency of screw loosening varies widely throughout the literature. Rates from 1% to 40% are reported [1–4] depending on age, bone quality, and number of fused levels [5]. However, in most reports, the judgment of screw fixation is based on plain radiograph assessment [6–11]. A radiolucent zone surrounding a pedicle screw can be a sign of screw loosening, but a loose screw is not always surrounded by a radiolucent zone [7]. Also, more than 50% of radiolucent zones can disappear within 2 years if detected within 6 months after operation [11]. However, radiolucent zones persisting for 2 years or longer after surgery are highly associated with pseudarthrosis [11].

Computed tomography (CT), particularly thin-section helical CT [12], is currently considered the diagnostic imaging modality of choice for detection of screw loosening and, potentially, pseudarthrosis, though screw loosening does not always imply pseudarthrosis. Recent studies have investigated the role of SPECT/CT in detecting spinal implant loosening with better accuracy though practicality and radiation exposure is a concern [13,14]. Magnetic resonance imaging (MRI), with the advantage of avoiding ionizing radiation and better soft tissue visualization [15], is increasingly used in assessment of a patient with spinal disorders. However, concomitant magnetic-susceptibility artifacts seen with metallic implants can hinder images [16,17]. Recent MRI advances and use of nonferromagnetic titanium implants has improved spinal images with hardware in place [18–21]. In turn, newer MRIs may prove a valuable option in detecting screw loosening.

Recent reports have shown promise using MRI and metal artifact reduction sequences of detection of implant loosening in the knee and hip [22–24]. Studies focusing on pedicle screw loosening are lacking. The aim of this study was to assess the sensitivity and specificity of the most commonly used imaged modalities (standard radiographs, CT, and MRI) in detection of pedicle screws loosening following an attempted posterior lumbar fusion.

## Material and methods

Ethical approval from the local ethics committee was obtained, and the study was registered at the Swiss National Clinical Trials Portal (registration number: SNCTP000000314).

### Study population

Forty-one patients (22 females, 19 males, mean age  $67.3 \pm 10.9$  years [range: 27–89]) were enrolled between August 2014 and April 2017 at a single institution with planned revision surgery for painful pseudoarthrosis, adjacent segment disease or proximal junction kyphosis. Further inclusion criteria were informed consent, age older than 18, and titanium instrumentation. The time interval between index surgery and revision surgery was  $3.05 \pm 3.12$  years (range: 0.06–13.50).

In total, 159 screws were examined with MRI, CT, and standard radiographs before intraoperatively quantifying each screw hold with a torque-measuring device. The time interval between the date of MRI, CT, and radiographs and date of revision surgery was  $36 \pm 40.7$  days (range: 1–157 days),  $48.7 \pm 58.78$  days (range: 1–304 days), and  $29.2 \pm 39.42$  (range: 0–188), respectively.

### MRI, CT, and radiographic protocol

All MRI scans were performed at the University Hospital Balgrist on a 1.5-T scanner (Magnetom Avanto, Siemens Healthcare, Erlangen, Germany). The software used was Syngo MR VD13, Siemens Healthcare. The following imaging sequences of lumbar MRI were employed: coronal short tau inversion recovery (STIR) WARP, transverse T2w turbo spin-echo (TSE) high bandwidth, sagittal T2w TSE high bandwidth, sagittal T1w TSE high bandwidth. WARP is defined as high receiver bandwidth of 610–620 Hz/px and view-angle tilting 100 %, and the STIR WARP sequence includes an optimized inversion pulse that adapted to the high receiver bandwidth [25].

All CT scans were performed on a 64-MDCT scanner (Brilliance, Philips Healthcare) using standard “bone” protocol (120 kV; 250 mAs with intensity modulation; 1 second rotation time; slice collimation,  $64 \times 0.625$  mm). Image reconstruction produced images with a slice thickness of 2 mm at a 1 mm increment. Automatic rigid image registration was performed using the SYNGO multimodality software (Siemens Healthcare, Germany).

Conventional lateral and anteroposterior radiographs were taken at least 6 months before revision surgery.

### Image analyses

All images were assessed separately by two well experienced musculoskeletal radiologists (Reader 1: R.S. senior consultant and Reader 2: N.F. consultant). Analyses of all image sets were performed by commercial Picture Archiving and Communication System viewer Merlin 5.2. (Phoenix-PACS, Freiburg, Germany).

The readers independently evaluated MRI, CT, and radiographs without knowledge of the intraoperative findings.

### MRI

Investigated signs of screw loosening in MRI were: presence of peri-screw edema (Readers 1 and 2) and size of peri-screw edema (Reader 2). Maximal width of each sign was recorded irrespective of the length (Fig. 1).

### CT and radiographs

Maximum size of peri-screw osteolysis if present, also known as radiolucent zones, was recorded irrespective of the length of the lucency and slice of occurrence in CT. The influence of these signs on screw torque was analyzed separately (Fig. 2).

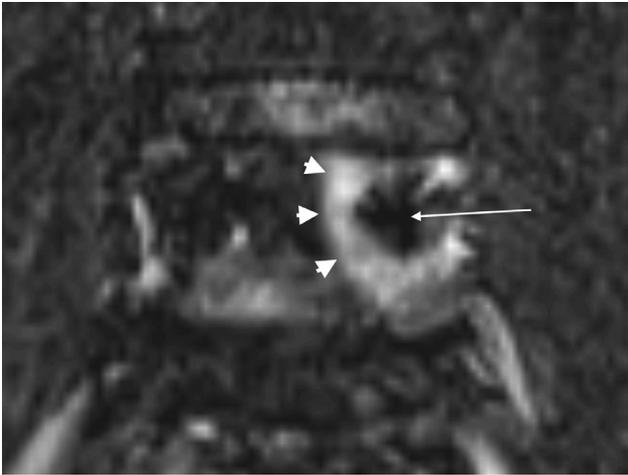


Fig. 1. MRI (coronal short tau inversion recovery [STIR] WARP) showing the pedicle screw (arrow) and peri-screw edema (arrowheads) as a screw loosening sign.

### Surgical protocol

All patients underwent revision surgery during which all pedicle screws hold was quantified. After exposing the implants, rods were removed separately, and screw heads were freed from soft tissue. A torque meter (Model TT03, Mark-10 Corporation, New York, USA) with an appropriate screwdriver (Fig. 3) was inserted and the maximum torque was measured while unscrewing the screw. Screws were then replaced, and the subsequent surgery was performed as usual and independent of the study.

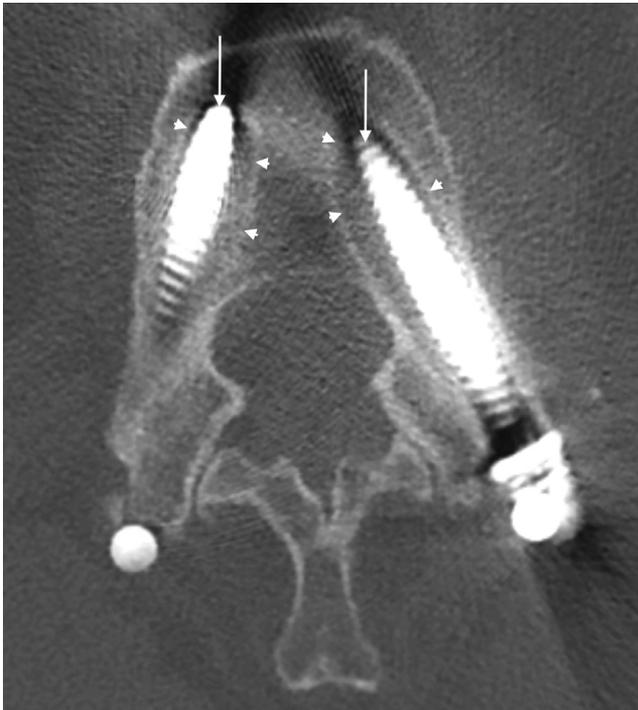


Fig. 2. Transverse CT showing two pedicle screws (arrow) with peri-screw osteolysis (arrowheads) as a screw loosening sign.



Fig. 3. Torque meter with exchangeable screwdriver for intraoperative screw torque measurement.

### Statistical analysis

All values are given as the mean  $\pm$  1 SD. Interrater reliability was assessed using two-way random effects single measures intraclass correlation (ICC (2,1)) for interval-scaled values and Cohens Kappa for nominal variables. Associations between interval-scaled radiographic predictor variables with screw loosening were investigated using separate ordinary least squares linear regressions including a constant of peri-screw osteolysis and size of edema on natural log-transformed torque values. A p value  $<$  .05 was considered statistically significant. All statistical analyses were performed with SPSS software (version 24.0; SPSS Inc., Chicago, IL, USA).

## Results

### Intraoperative measures

The overall screw torque force was  $144.5 \pm 131.7$  Ncm (range: 0–500 Ncm). Screw loosening was defined as a screw torque  $<$  60 Ncm since the distribution of screw torques seems to contain two overlapping normal distributions, one for loosened screws (mean:  $13.4 \pm 17.3$  Ncm) and one for firm screws ( $161.9 \pm 85.9$  Ncm) with an intersection point at 60 Ncm (Fig. 4). Fifty-five loosened screws ( $<$  60 Ncm) and 104 firm screws ( $>$  60 Ncm) were identified.

### Analysis of peri-screw osteolysis in radiographs

Linear regression analysis of the radiographic score on ln-transformed (natural logarithm) torque values revealed a significant ( $p < .001$ ) negative association of peri-screw osteolysis with torque (Fig. 5) in the form:  $\text{Torque} = e^{5.015 - 0.574 * \text{RadScore}}$ .  $R^2$  was 0.166. This readout was only done by one reader (reader 1) since the role of radiographs in detecting screw loosening has already been previously examined [7].

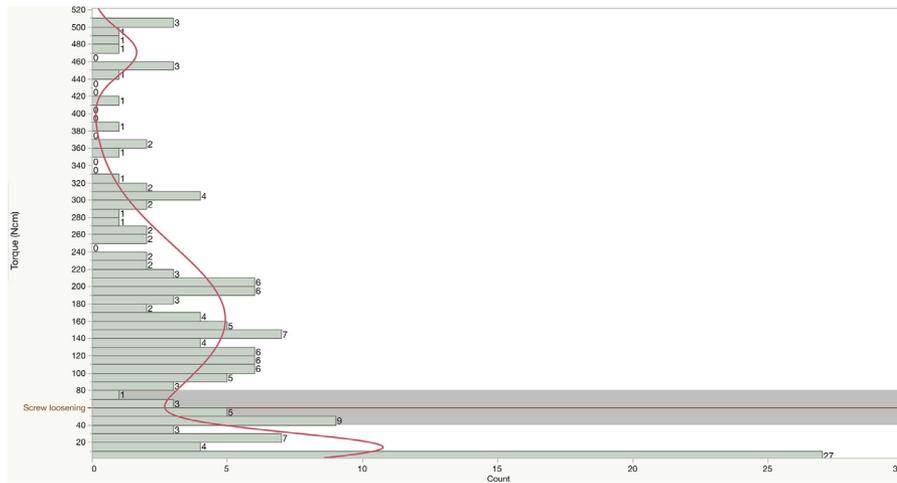


Fig. 4. Distribution of screw torques shows an intersection point of two overlapping normal distributions at 60 Ncm. Screw loosening was therefore defined as a screw torque <60 Ncm. However, there might be a transition zone between loosened screw and firm screw shown (gray zone: 60 Ncm±20 Ncm).

*Analysis of peri-screw osteolysis in CT*

For both readers, linear regression analysis of the radiographic score on ln-transformed torque values revealed a significant (p<.001) negative association of peri-screw osteolysis with torque (Fig. 6) in the form: Torque = e<sup>4.975-0.553\*RadScore</sup> (Reader 1) and Torque = e<sup>4.950-0.445\*RadScore</sup> (Reader 2). R<sup>2</sup> was 0.229 and 0.240, respectively. Intraclass correlation analysis for detecting radiolucent zones in a CT yielded good agreement of ICC = 0.860 (p<.001) in a two-way random effects model on a single measures approach.

*Analysis of peri-screw bone edema in MRI*

For both readers, presence of bone edema was significantly associated with a lower mean unscrew torque force (Fig. 7). For reader 1 mean unscrew torque without presence of bone edema was 159.45±132.32 Ncm versus 69.81±110.49 Ncm with presence of bone edema (p=.001).

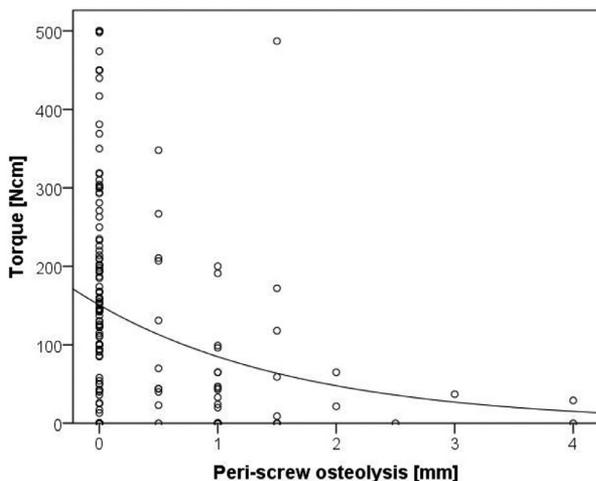


Fig. 5. Linear regression analysis of peri-screw osteolysis in radiographs with ln-transformed torque values shows a significant negative association.

Similar results were measured by reader 2: 177.45±132.34 Ncm versus 21.78±23.03 Ncm, respectively (p<.001).

Cohen’s Kappa revealed, however, a poor agreement between the two raters concerning presence of edema around the screw (k=0.289, p<.001). There was agreement for 180 screws and no agreement in 43 screws. Linear regression analysis of the radiographic score on ln-transformed torque values revealed a significant (p<.001) negative association of edema size with torque in the form: Torque = e<sup>5.144-0.126\*RadScore</sup>. R<sup>2</sup> was 0.062.

*Sensitivity and specificity of each radiological modality*

Because there might be no sharp cutoff torque for a loose screw, we also analyzed 80 Ncm and 40 Ncm as a cutoff to test for hypothesis stability. However, this had little effect on sensitivity and specificity in any modality (Table 1).

With a cutoff torque at 60 Ncm, the highest sensitivity was achieved by peri-screw osteolysis in CT (52.4%–64.8%), followed by peri-screw osteolysis in radiographs (54.2%). Sensitivity of MRI (34.5%–43.9%) was inferior to both, CT and radiographs.

Both readers achieved an excellent specificity using the modality peri-screw osteolysis in CT (97.8%–100%), whereas radiographs and MRI achieved lower values (83.5% and 77.4%–92.1%). Overall, peri-screw osteolysis in CT achieved best values with however an unacceptable sensitivity but good specificity (64.8% and 96.7%, respectively) (Table 1).

**Discussion**

The aim of this study was to assess the sensitivity and specificity of the most commonly used imaged modalities (standard radiograph, CT, and MRI) in detection of pedicle screws loosening within a prospective trial with intraoperative quantification of screw loosening. Our results confirm that peri-screw osteolysis in CT is still the best indicator for screw-loosening after spinal fusion. However, the

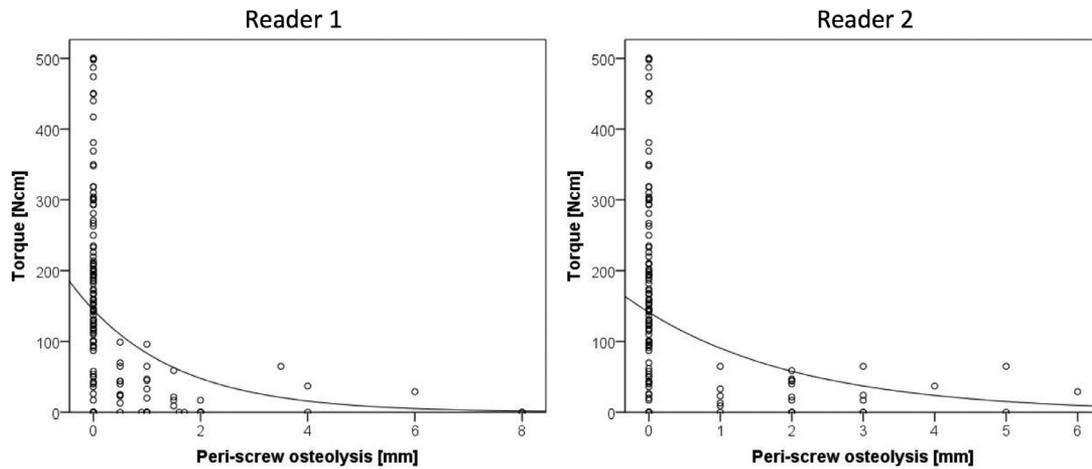


Fig. 6. Linear regression analysis of peri-screw osteolysis in CT with ln-transformed torque values. There is a significant negative association in both readers with good interclass correlation.

maximum sensitivity and specificity was 64.8% and 96.7% for CT, 54.2% and 83.5% for radiographs, and 43.9% and 92.1% for MRI, respectively.

These results indicate that none of the modalities are sufficiently sensitive in detecting screw loosening, though CT seems to have reasonable specificity of screw loosening. In other words, if the CT shows peri-screw osteolysis, the screw is most likely loose. Sanden et al. reported similar results with 64% sensitivity and 100% specificity for radiographs using intraoperative screw torque measurement as the gold standard [7]. To the authors’ knowledge, there are no prior studies comparing CT with intraoperative torque as a reference. However, CT has been reported to be more sensitive than radiographs for detecting screw loosening [26,27].

Disadvantages of CT are high radiation exposure and its reduced ability to define soft tissues pathologies such as nerve compression, infections, scar tissue, bone edema, and intradural pathologies compared with MRI [28–31]. Therefore, MRI is often indispensable in the investigation of ongoing symptoms following spinal fusion.

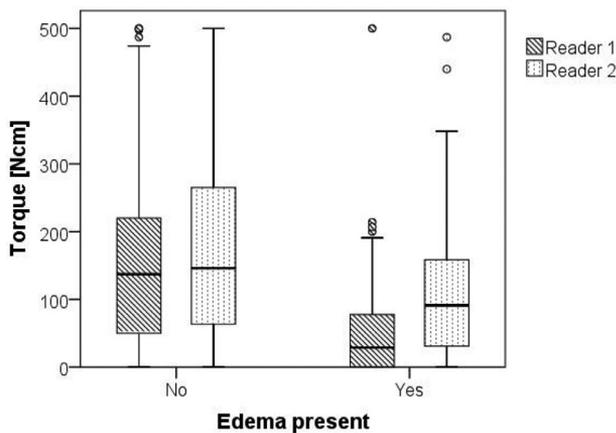


Fig. 7. Mean unscrew torques for both, screws with and without peri-screw edema in MRI. For both readers, there was a significant reduction of unscrew torque in cases with peri-screw edema.

To the best knowledge of the authors, this is the first study investigating the role of MRI in detection of screw loosening. Previous studies have shown that postoperative MRI’s with metal artifact reduction techniques including high bandwidth optimization, view angle tilting, multispectral imaging techniques multiacquisition variable resonance image combination, and slice-encoding for metal artifact correction may significantly reduce metal-induced artifacts and reliably improve visibility of anatomical structures such as the dural sac, nerve roots and bone–implant interface [25,32]. These techniques require significantly longer acquisition times and may not be feasible on a routine basis [33]. Therefore, we investigated in this study TSE with high bandwidth optimization and STIR WARP sequences that are known to have reasonable acquisition times. However, it remains unknown if sensitivity and specificity of MRI for detecting screw loosening would be improved using sequences with more acquisition time such as slice-encoding for metal artifact or multiacquisition variable resonance image combination [20,22,23,25,34].

The focus of the study question was specifically to define sensitivity and specificity of current imaging modalities such as MRI, CT, and radiographs in detecting screw loosening. Inclusion criteria were therefore not reduced to patients suspected of painful pseudoarthrosis but all kind of indications for revision surgery after spinal fusion. We do not claim to report differentiation of the proportions of patients suffering from isolated pseudoarthrosis versus so-called painful screw loosening. It is, however, evident from a prior study that screw loosening is strongly associated with pseudoarthrosis when still present two years after surgery and that signs of screw loosening are seen in 93.3% of pseudoarthrosis [11]. Other signs, such as absence of fusion mass or osteolysis and edema around the intervertebral cage, can suggest pseudoarthrosis. These were not analyzed in this study.

Despite its role in the evaluation of postoperative lumbar fusion patients, MRI has had little role in detecting

Table 1  
Sensitivity and specificity of different diagnostic modalities with varying definitions of a loose screw (<40 Ncm, <60 Ncm, and <80 Ncm)

Predictor		Torque				Torque				Torque			
		<80 Ncm		>80 Ncm		<60 Ncm		>60 Ncm		<40 Ncm		>40 Ncm	
		Count	Spec.	Sens.	Spec.	Count	Spec.	Sens.	Spec.	Count	Spec.	Sens.	Spec.
Peri-screw osteolysis radiographs (Reader 1)	No instability predicted	22		81		22		81		16		87	
	Instability predicted	30	57.7%	12	87.1%	26	83.5%	16	54.2%	20	83.5%	22	55.6%
Peri-screw osteolysis CT (Reader 1)	No instability predicted	19		91		19		91		13		97	
	Instability predicted	39	67.2%	2	97.8%	35	93.8%	6	64.8%	30	93.8%	11	69.8%
Peri-screw osteolysis CT (Reader 2)	No instability predicted	22		85		20		87		13		94	
	Instability predicted	25	53.2%	0	100.0%	22	96.7%	3	52.4%	18	96.7%	7	58.1%
Peri-screw edema MRI (Reader 1)	No instability predicted	39		90		36		93		28		101	
	Instability predicted	20	33.9%	7	92.8%	19	92.1%	8	34.5%	15	92.1%	12	34.9%
Peri-screw edema MRI (Reader 2)	No instability predicted	27		68		23		72		17		78	
	Instability predicted	19	41.3%	20	77.3%	18	77.4%	21	43.9%	13	77.4%	26	43.3%

pseudoarthrosis [35,36]. Computed tomography has been reported to be the most accurate modality [15,37], though intraoperative detection of pseudoarthrosis remains the gold standard [38,39].

Several other limitations need consideration if interpreting the here presented results. As shown in our study there seems to be no sharp screw torque cutoff that defines a loose screw. We did find an exponential relationship between screw torque and several loosening signs. This contrasts with the study by Sanden et al. [7], which defined 40 Ncm as a cutoff since no extraction torques between 40 and 75 Ncm were found. We could not detect such a clear gap in our data. However, there seemed to be two normal distributions, one of loosened screws and one of clearly firm screws with an intersection point around 60 Ncm. We therefore set our cutoff torque at 60 Ncm and compared this with other cutoff torques at 80 Ncm and 40 Ncm. Little change in sensitivity and specificity of each image modality was observed with this variation. A further limitation of this study is that only titanium-based implants were included. Because metal artifacts are much more extensive with other materials such as cobalt-chromium or stainless-steel [18,40–42], our results may not applicable to these materials.

Finally, it could be questioned if measurement of unscrew torque is the right parameter to determine screw loosening and whether pullout strength might be more suitable to define screw loosening. Several studies have shown that insertional torque does not necessarily correlate with axial pullout force and both parameters might be influenced by different factors [43–45]. Neither axial pullout force nor unscrew torque seems to adequately mimic physiological loading [44,46–49]. However, in vivo experiments allow only for unscrew torque measurements since both toggling and pullout experiments have a destructive nature that are not ideal for patients. There seems to be, nonetheless, some correlation between screw torque and the number of toggling cycles until failure occurs [44]. As far as the authors are aware, screw torque is the only intraoperative measurable parameter to quantify the screw–bone interface hold for in vivo human studies.

### Conclusions

Standard radiographs, CT, or MRI are highly sensitive in detection of pedicle screw loosening. Computed tomography remains the most specific image modality for screw loosening.

### References

- [1] Ohlin A, Karlsson M, Düppe H, Hasserius R, Redlund-Johnell I. Complications after transpedicular stabilization of the spine. A survivorship analysis of 163 cases. *Spine (Phila Pa 1976)* 1994;19:2774–9.
- [2] Sandén B, Olerud C, Petré-Mallmin M, Larsson S. Hydroxyapatite coating improves fixation of pedicle screws. A clinical study. *J Bone Joint Surg Br* 2002;84:387–91.

- [3] Sandén B, Olerud C, Johansson C, Larsson S. Improved bone-screw interface with hydroxyapatite coating: an in vivo study of loaded pedicle screws in sheep. *Spine (Phila Pa 1976)* 2001;26:2673–8.
- [4] Pihlajämäki H, Myllynen P, Böstman O. Complications of transpedicular lumbosacral fixation for non-traumatic disorders. *J Bone Joint Surg Br* 1997;79:183–9.
- [5] Galbusera F, Volkheimer D, Reitmaier S, Berger-Roscher N, Kienle A, Wilke H-J. Pedicle screw loosening: a clinically relevant complication? *Eur Spine J* 2015;24:1005–16. doi: [10.1007/s00586-015-3768-6](https://doi.org/10.1007/s00586-015-3768-6).
- [6] Sandén B, Olerud C, Larsson S, Robinson Y. Insertion torque is not a good predictor of pedicle screw loosening after spinal instrumentation: a prospective study in 8 patients. *Patient Saf Surg* 2010;4:14. doi: [10.1186/1754-9493-4-14](https://doi.org/10.1186/1754-9493-4-14).
- [7] Sandén B, Olerud C, Petré-Mallmin M, Johansson C, Larsson S. The significance of radiolucent zones surrounding pedicle screws. Definition of screw loosening in spinal instrumentation. *J Bone Joint Surg Br* 2004;86:457–61.
- [8] Okuyama K, Abe E, Suzuki T, Tamura Y, Chiba M, Sato K. Can insertional torque predict screw loosening and related failures? An in vivo study of pedicle screw fixation augmenting posterior lumbar interbody fusion. *Spine (Phila Pa 1976)* 2000;25:858–64.
- [9] Mizuno K, Shinomiya K, Nakai O, Shindo S, Otani K. Intraoperative insertion torque of lumbar pedicle screw and postoperative radiographic evaluation: short-term observation. *J Orthop Sci* 2005;10:137–44. doi: [10.1007/s00776-004-0873-5](https://doi.org/10.1007/s00776-004-0873-5).
- [10] Ozawa T, Takahashi K, Yamagata M, Ohtori S, Aoki Y, Saito T, et al. Insertional torque of the lumbar pedicle screw during surgery. *J Orthop Sci* 2005;10:133–6. doi: [10.1007/s00776-004-0883-3](https://doi.org/10.1007/s00776-004-0883-3).
- [11] Tokuhashi Y, Matsuzaki H, Oda H, Uei H. Clinical course and significance of the clear zone around the pedicle screws in the lumbar degenerative disease. *Spine (Phila Pa 1976)* 2008;33:903–8. doi: [10.1097/BRS.0b013e318161eff](https://doi.org/10.1097/BRS.0b013e318161eff).
- [12] Cook SD, Patron LP, Christakis PM, Bailey KJ, Banta C, Glazer PA. Comparison of methods for determining the presence and extent of anterior lumbar interbody fusion. *Spine (Phila Pa 1976)* 2004;29:1118–23.
- [13] Rager O, Schaller K, Payer M, Tchermir D, Ratib O, Tessitore E. SPECT/CT in differentiation of pseudarthrosis from other causes of back pain in lumbar spinal fusion. *Clin Nucl Med* 2012;37:339–43. doi: [10.1097/RLU.0b013e318239248b](https://doi.org/10.1097/RLU.0b013e318239248b).
- [14] Hudyana H, Maes A, Vandenberghe T, Fidlers L, Sathekge M, Nicolai D, et al. Accuracy of bone SPECT/CT for identifying hardware loosening in patients who underwent lumbar fusion with pedicle screws. *Eur J Nucl Med Mol Imaging* 2016;43:349–54. doi: [10.1007/s00259-015-3158-7](https://doi.org/10.1007/s00259-015-3158-7).
- [15] Tohtz SW, Rogalla P, Taupitz M, Perka C, Winkler T, Putzier M. Inter- and intraobserver variability in the postoperative evaluation of transpedicular stabilization: computed tomography versus magnetic resonance imaging. *Spine J* 2010;10:285–90. doi: [10.1016/j.spinee.2009.12.020](https://doi.org/10.1016/j.spinee.2009.12.020).
- [16] Jinkins JR, Van Goethem JWM. The postsurgical lumbosacral spine. *Radiol Clin North Am* 2001;39:1–29. doi: [10.1016/S0033-8389\(05\)70261-X](https://doi.org/10.1016/S0033-8389(05)70261-X).
- [17] Berquist TH. Imaging of the postoperative spine. *Radiol Clin North Am* 2006;44:407–18. doi: [10.1016/j.rcl.2006.01.002](https://doi.org/10.1016/j.rcl.2006.01.002).
- [18] Koch KM, Hargreaves BA, Pauly KB, Chen W, Gold GE, King KF. Magnetic resonance imaging near metal implants. *J Magn Reson Imaging* 2010;32. doi: [10.1002/jmri.22313](https://doi.org/10.1002/jmri.22313).
- [19] Viano AM, Gronemeyer SA, Haliloglu M, Hoffer FA. Improved MR imaging for patients with metallic implants. *Magn Reson Imaging* 2000;18:287–95.
- [20] Jungmann PM, Agten CA, Pfirrmann CW, Sutter R. Advances in MRI around metal. *J Magn Reson Imaging* 2017;46:972–91. doi: [10.1002/jmri.25708](https://doi.org/10.1002/jmri.25708).
- [21] Lu W, Pauly KB, Gold GE, Pauly JM, Hargreaves BA. SEMAC: slice encoding for metal artifact correction in MRI. *Magn Reson Med* 2009;62:66–76. doi: [10.1002/mrm.21967](https://doi.org/10.1002/mrm.21967).
- [22] Sutter R, Ulbrich EJ, Jellus V, Nittka M, Pfirrmann CWA. Reduction of metal artifacts in patients with total hip arthroplasty with slice-encoding metal artifact correction and view-angle tilting MR imaging. *Radiology* 2012;265:204–14. doi: [10.1148/radiol.12112408](https://doi.org/10.1148/radiol.12112408).
- [23] Sutter R, Hodek R, Fucentese SF, Nittka M, Pfirrmann CWA. Total knee arthroplasty MRI featuring slice-encoding for metal artifact correction: reduction of artifacts for STIR and proton density-weighted sequences. *Am J Roentgenol* 2013;201:1315–24. doi: [10.2214/AJR.13.10531](https://doi.org/10.2214/AJR.13.10531).
- [24] Agten CA, Del Grande F, Fucentese SF, Blatter S, Pfirrmann CWA, Sutter R. Unicompartamental knee arthroplasty MRI: impact of slice-encoding for metal artefact correction MRI on image quality, findings and therapy decision. *Eur Radiol* 2015;25:2184–93. doi: [10.1007/s00330-015-3596-4](https://doi.org/10.1007/s00330-015-3596-4).
- [25] Ulbrich EJ, Sutter R, Aguiar RF, Nittka M, Pfirrmann CW. STIR sequence with increased receiver bandwidth of the inversion pulse for reduction of metallic artifacts. *Am J Roentgenol* 2012;199:W735–42. doi: [10.2214/AJR.11.8233](https://doi.org/10.2214/AJR.11.8233).
- [26] Ohtori S, Inoue G, Orita S, Yamauchi K, Eguchi Y, Ochiai N, et al. Comparison of teriparatide and bisphosphonate treatment to reduce pedicle screw loosening after lumbar spinal fusion surgery in postmenopausal women with osteoporosis from a bone quality perspective. *Spine (Phila Pa 1976)* 2013;38:E487–92. doi: [10.1097/BRS.0b013e31828826dd](https://doi.org/10.1097/BRS.0b013e31828826dd).
- [27] Abul-Kasim K, Ohlin A. Evaluation of implant loosening following segmental pedicle screw fixation in adolescent idiopathic scoliosis: a 2 year follow-up with low-dose CT. *Scoliosis* 2014;9:13. doi: [10.1186/1748-7161-9-13](https://doi.org/10.1186/1748-7161-9-13).
- [28] Rausch V, Bannas P, Schoen G, Froelich A, Well L, Regier M, et al. Diagnostic yield of multidetector computed tomography in patients with acute spondylodiscitis. *RöFo – Fortschr Geb Röntgenstrahlen Bildgeb Verfahr* 2017;189:339–46. doi: [10.1055/s-0043-101864](https://doi.org/10.1055/s-0043-101864).
- [29] van Rijn RM, Wassenaar M, Verhagen AP, Ostelo RWJG, Ginai AZ, de Boer MR, et al. Computed tomography for the diagnosis of lumbar spinal pathology in adult patients with low back pain or sciatica: a diagnostic systematic review. *Eur Spine J* 2012;21:228–39. doi: [10.1007/s00586-011-2012-2](https://doi.org/10.1007/s00586-011-2012-2).
- [30] Notohamiprodjo S, Stahl R, Braunagel M, Kazmierczak PM, Thierfelder KM, Treitl KM, et al. Diagnostic accuracy of contemporary multidetector computed tomography (MDCT) for the detection of lumbar disc herniation. *Eur Radiol* 2017;27:3443–51. doi: [10.1007/s00330-016-4686-7](https://doi.org/10.1007/s00330-016-4686-7).
- [31] Yi JS, Cha JG, Han JK, Kim H-J. Imaging of herniated discs of the cervical spine: inter-modality differences between 64-slice multidetector CT and 1.5-T MRI. *Korean J Radiol* 2015;16:881. doi: [10.3348/kjr.2015.16.4.881](https://doi.org/10.3348/kjr.2015.16.4.881).
- [32] Song KD, Yoon YC, Park J. Reducing metallic artefacts in post-operative spinal imaging: slice encoding for metal artefact correction with dual-source parallel radiofrequency excitation MRI at 3.0T. *Br J Radiol* 2013;86:20120524. doi: [10.1259/bjr.20120524](https://doi.org/10.1259/bjr.20120524).
- [33] Hargreaves BA, Chen W, Lu W, Alley MT, Gold GE, Brau ACS, et al. Accelerated slice encoding for metal artifact correction. *J Magn Reson Imaging* 2010;31:987–96. doi: [10.1002/jmri.22112](https://doi.org/10.1002/jmri.22112).
- [34] Do T, Sutter R, Skornitzke S, Weber M-A. CT and MRI techniques for imaging around orthopedic hardware. *RöFo – Fortschritte Auf Dem Gebiet Der Röntgenstrahlen Und Der Bildgeb Verfahren* 2017. doi: [10.1055/s-0043-118127](https://doi.org/10.1055/s-0043-118127).
- [35] Lang P, Chafetz N, Genant HK, Morris JM. Lumbar spinal fusion. Assessment of functional stability with magnetic resonance imaging. *Spine (Phila Pa 1976)* 1990;15:581–8.
- [36] Choudhri TF, Mummaneni PV, Dhall SS, Eck JC, Groff MW, Ghogawala Z, et al. Guideline update for the performance of fusion procedures for degenerative disease of the lumbar spine. Part 4: radiographic assessment of fusion status. *J Neurosurg Spine* 2014;21:23–30. doi: [10.3171/2014.4.SPINE14267](https://doi.org/10.3171/2014.4.SPINE14267).

- [37] Kosmopoulos V, Schizas C. Pedicle screw placement accuracy. *Spine (Phila Pa 1976)* 2007;32:E111–20. doi: [10.1097/01.brs.0000254048.79024.8b](https://doi.org/10.1097/01.brs.0000254048.79024.8b).
- [38] Quon A, Dodd R, Iagaru A, de Abreu MR, Hennemann S, Alves Neto JM, et al. Initial investigation of <sup>18</sup>F-NaF PET/CT for identification of vertebral sites amenable to surgical revision after spinal fusion surgery. *Eur J Nucl Med Mol Imaging* 2012;39:1737–44. doi: [10.1007/s00259-012-2196-7](https://doi.org/10.1007/s00259-012-2196-7).
- [39] Brans B, Weijers R, Halders S, Wierts R, Peters M, Punt I, et al. Assessment of bone graft incorporation by 18F-fluoride positron-emission tomography/computed tomography in patients with persisting symptoms after posterior lumbar interbody fusion. *EJNMMI Res* 2012;2:42. doi: [10.1186/2191-219X-2-42](https://doi.org/10.1186/2191-219X-2-42).
- [40] Lee M-J, Kim S, Lee S-A, Song H-T, Huh Y-M, Kim D-H, et al. Overcoming artifacts from metallic orthopedic implants at high-field-strength MR imaging and multi-detector CT. *Radiographics* 2007;27:791–803. doi: [10.1148/rg.273065087](https://doi.org/10.1148/rg.273065087).
- [41] Harris CA, White LM. Metal artifact reduction in musculoskeletal magnetic resonance imaging. *Orthop Clin North Am* 2006;37:349–59. doi: [10.1016/j.jocl.2006.04.001](https://doi.org/10.1016/j.jocl.2006.04.001).
- [42] White LM, Buckwalter KA. Technical considerations: CT and MR imaging in the postoperative orthopedic patient. *Semin Musculoskelet Radiol* 2002;6:5–17. doi: [10.1055/s-2002-23160](https://doi.org/10.1055/s-2002-23160).
- [43] Kwok AW, Finkelstein JA, Woodside T, Hearn TC, Hu RW. Insertional torque and pull-out strengths of conical and cylindrical pedicle screws in cadaveric bone. *Spine (Phila Pa 1976)* 1996;21:2429–34.
- [44] Zdeblick TA, Kunz DN, Cooke ME, McCabe R. Pedicle screw pull-out strength. Correlation with insertional torque. *Spine (Phila Pa 1976)* 1993;18:1673–6.
- [45] Inceoglu S, Ferrara L, McLain RF. Pedicle screw fixation strength: pullout versus insertional torque. *Spine J* 2004;4:513–8. doi: [10.1016/j.spinee.2004.02.006](https://doi.org/10.1016/j.spinee.2004.02.006).
- [46] Law M, Tencer AF, Anderson PA. Caudo-cephalad loading of pedicle screws: mechanisms of loosening and methods of augmentation. *Spine (Phila Pa 1976)* 1993;18:2438–43.
- [47] Rohlmann A, Graichen F, Weber U, Bergmann G. 2000 Volvo award winner in biomechanical studies: monitoring in vivo implant loads with a telemeterized internal spinal fixation device. *Spine (Phila Pa 1976)* 2000;25:2981–6.
- [48] Goel VK, Winterbottom JM, Weinstein JN. A method for the fatigue testing of pedicle screw fixation devices. *J Biomech* 1994;27:1383–8.
- [49] Mehmanparast H, Petit Y, Mac-Thiong J-M. Comparison of pedicle screw loosening mechanisms and the effect on fixation strength. *J Biomech Eng* 2015;137:121003. doi: [10.1115/1.4031821](https://doi.org/10.1115/1.4031821).