



Assessment of left atrial volume in dogs: comparisons of two-dimensional and real-time three-dimensional echocardiography with ECG-gated multidetector computed tomography angiography^{☆, ☆ ☆}



Jonathan Bouvard, DVM^{*}, Florence Thierry, DVM,
Geoffrey J. Culshaw, BVMS, PhD, Tobias Schwarz, DVM,
Ian Handel, BVSc, MSci, PhD, Yolanda Martinez Pereira,
Lda Vet

*The Royal (Dick) School of Veterinary Studies, Division of Clinical Veterinary Sciences,
University of Edinburgh, Edinburgh, UK*

Received 17 November 2018; received in revised form 2 June 2019; accepted 13 June 2019

KEYWORDS

Canine;
Cardiac volumes;

Abstract *Introduction:* We hypothesized that real-time three-dimensional echocardiography (RT-3DE) was superior to two-dimensional echocardiography for the estimation of left atrial volume (LAV), using electrocardiographic (ECG)-gated

Results were presented at the 28th congress of the European College of Veterinary Internal Medicine Companion Animals, Rotterdam, the Netherlands, 2018.

^{*} A unique aspect of the Journal of Veterinary Cardiology is the emphasis of additional web-based images permitting the detailing of procedures and diagnostics. These images can be viewed (by those readers with subscription access) by going to <http://www.sciencedirect.com/science/journal/17602734>. The issue to be viewed is clicked and the available PDF and image downloading is available via the Summary Plus link. The supplementary material for a given article appears at the end of the page. Downloading the videos may take several minutes. Readers will require at least Quicktime 7 (available free at <http://www.apple.com/quicktime/download/>) to enjoy the content. Another means to view the material is to go to <http://www.doi.org> and enter the doi number unique to this paper which is indicated at the end of the manuscript.

^{**} A unique aspect of the Journal of Veterinary Cardiology is the emphasis of additional web-based materials permitting the detailing of procedures and diagnostics. These materials can be viewed (by those readers with subscription access) by going to <http://www.sciencedirect.com/science/journal/17602734>. The issue to be viewed is clicked and the available PDF and image downloading is available via the Summary Plus link. The supplementary material for a given article appears at the end of the page. To view the material is to go to <http://www.doi.org> and enter the doi number unique to this paper which is indicated at the end of the manuscript.

^{*} Corresponding author.

E-mail address: j.bouvard@ed.ac.uk (J. Bouvard).

<https://doi.org/10.1016/j.jvc.2019.06.004>

1760-2734/© 2019 Elsevier B.V. All rights reserved.

Biplane-modified simpson method;
Biplane area-length method;
Advanced cardiac imaging

multidetector computed tomography angiography (MDCTA) as a volumetric gold standard. The aim was to compare maximum LAV (LAV_{max}) and minimum LAV (LAV_{min}) measured by biplane area-length method (ALM), biplane method of disk (MOD) and RT-3DE with 64-slice ECG-gated MDCTA in dogs

Animals: The study included twenty dogs, anaesthetized for various diagnostic purposes and without evidence of cardiovascular disease.

Methods: Left atrial volume was estimated by ALM, MOD and RT-3DE following ECG-gated MDCTA. The results were compared with LAV from MDCTA and correlations were performed. The limits of agreement (LoA) between methods were evaluated using Bland–Altman analysis and intraclass correlations. Coefficients of variation were calculated.

Results: Area-length method ($r = 0.79$ and 0.72), MOD ($r = 0.81$ and 0.70) and RT-3DE ($r = 0.94$ and 0.82) correlated with MDCTA for LAV_{max} and LAV_{min} , respectively (all $p < 0.05$). Biases for LAV_{max} (-0.96 mL, 95% LoA: -5.6 to 3.7) and LAV_{min} (-0.67 mL, 95% LoA: -5.4 – 4.1) were minimal with RT-3DE, reflecting a slight underestimation. Conversely, MOD (LAV_{max} bias = 3.19 mL, 95% LoA: -5.7 – 12.1 ; LAV_{min} bias = 1.96 mL, 95% LoA: -4.6 – 8.5) and ALM (LAV_{max} bias = 4.05 , 95% LoA: -5.7 – 13.8 ; LAV_{min} bias = 2.80 mL, 95% LoA: -3.9 – 9.5) suggested LAV overestimation. Intraobserver and interobserver variability were adequate.

Conclusions: Real-time three-dimensional echocardiography is a non-invasive, accurate and feasible method with superior accuracy to two-dimensional methods.

© 2019 Elsevier B.V. All rights reserved.

Abbreviations

2D	two-dimensional
3D	three-dimensional
ALM	area-length method
CI	confidence intervals
ECG	electrocardiographic
ICC	intraclass correlation coefficient
LA	left atrium
LAV	left atrial volume
LAV _{max}	maximum left atrial volume
LAV _{min}	minimum left atrial volume
LoA	limits of agreement
MDCTA	multidetector computed tomography angiography
MOD	method of disk
RT-3DE	real-time three-dimensional echocardiography

Introduction

Left atrial size is a clinically useful measurement in left-sided cardiac disease and is acknowledged as a predictor of morbidity and mortality in human and veterinary medicine [1–5]. Left atrial size is routinely measured clinically with two-dimensional (2D) transthoracic echocardiography at ventricular end-systole or early diastole and indexed to aortic root (short axis) [6–8]. However,

the left atrium (LA) is a three-dimensional (3D) structure with complex geometry, and because LA enlargement may occur non-uniformly in a number of directions (craniocaudal, mediolateral and ventrodorsal) [9,10], uniplanar assessment of its size may be unreliable. It has been suggested that measurement of left atrial volume (LAV) on 2D echocardiography reduces these errors [11]. The American Society of Echocardiography recommends calculating LAV either by the disc summation algorithm (method of disk [MOD]), which is similar to the method for measuring left ventricular volume, or by an ellipsoid geometric model using the LA areas and lengths (area-length method [ALM]). Both techniques require two non-foreshortened left apical orthogonal views (two-chamber and four-chamber views) and are dependent on mathematical assumptions based on the LA having a fixed shape. Consequently, they systematically underestimate LAV in people [12–15]. This has been overcome by the advent of new 3D imaging modalities such as real-time 3D echocardiography (RT-3DE) [16–20], electrocardiographic (ECG)-gated multidetector computed tomography angiography (MDCTA) [13,21–25] and cardiac magnetic resonance imaging [12,25–27]. Left atrial volume obtained by 2D echocardiography offers limited accuracy. This is due to its reliance on geometric assumptions and the dependency on the view. To avoid LA foreshortening, two-chamber and four-chamber

views should be truly orthogonal and optimized to maximize LA length and base in each view. Unlike 2D echocardiography, RT-3DE includes the entire LA within the 3D volume data set and therefore is not subject to foreshortening, eliminates the limitations of geometric assumptions and thus reduces errors in volumetric measurement [10].

Furthermore, RT-3DE has good spatial and temporal resolution and, in people, has a greater correlation than its 2D counterpart with both ECG-gated cardiac magnetic resonance imaging and MDCTA, the current gold standards in volumetric measurement [12,24,25,27]. The introduction of new RT-3D transducers has resulted in sufficiently high frame rate image acquisition for veterinary clinical applications. Equally, postprocessing analysis software using semiautomated border detection algorithms minimizes the initial learning curve and facilitates analysis [28,29]. However, to date, RT-3DE assessment of LAV has only been validated in veterinary cardiology in one study including six healthy dogs [30].

We hypothesized that RT-3DE is more accurate than 2D echocardiography at calculating canine LAV. To investigate this hypothesis, we compared maximum LAV (LAV_{max}) and minimum LAV (LAV_{min}), measured by biplane ALM, biplane MOD and RT-3DE, with 64-slice ECG-gated MDCTA in dogs. Correlations between data sets were calculated, and intraobserver and interobserver variability in these methods were also determined.

Animals, materials and methods

Enrolment

This was a prospective study approved by our local ethics committee (Approval 45.17) and conducted at the Royal (Dick) School of Veterinary Studies between June 2017 and December 2017. Client-owned dogs were considered for enrolment if they had no history of cardiovascular disease and had been referred and scheduled for thoracic MDCTA under general anaesthesia. Informed client consent was obtained for every dog. Dogs were excluded if a murmur, arrhythmia or gallop rhythm was auscultated on physical examination. Dogs underwent oscillometric systolic blood pressure measurement^a and blood sampling for routine haematology and serum biochemistry and were anaesthetized using a standard protocol determined by a board-certified

anaesthetist based on individual patient requirements. Premedicants included acepromazine^b, partial^c or full^d opioid agonists and dexmedetomidine^e. Anaesthesia was induced by intravenous propofol^f and maintained following endotracheal intubation by isoflurane^g in oxygen. Electrocardiographic-gated MDCTA was performed, followed immediately by transthoracic echocardiography. Dogs were further excluded if a thoracic mass was seen to compress or displace the heart on ECG-gated MDCTA or if congenital or acquired cardiac disease was detected on echocardiography. Mild valvular insufficiencies, in the absence of chamber enlargement, were permitted.

Echocardiography

Echocardiography^h was performed under general anaesthesia by a single resident in cardiopulmonary medicine (J.B.), under the supervision of a board-certified cardiologist. Images were obtained with 4V-D (1.5–4.0 MHz)ⁱ and M5S-D (1.5–4.6 MHz)^j matrix phased array transducers during continuous ECG recording. Dogs were positioned alternatively in right and left lateral recumbency for transthoracic 2D, M-mode, pulsed-wave and continuous-wave Doppler studies and RT-3DE in accordance with the recommendations of the Echocardiography Committee of the Specialty of Cardiology of the American College of Veterinary Internal Medicine [31] and the American Society of Echocardiography [10,32]. Images were digitally stored and analyzed offline with commercially available software^k.

Electrocardiographic-gated MDCTA image acquisition

All MDCTA examinations were performed using a helical acquisition on a 64-slice MDCTA scanner^l. A transverse plane examination of the thorax was performed using 2-mm slice thickness and 1-mm

^b Acecare, Animalcare limited, United Kingdom.

^c Alvegesic, Dechra Veterinary products, United Kingdom.

^d Comfortan, Dechra Veterinary products, United Kingdom.

^e Dexmedetomidine, Orion Pharma, Turku, Finland.

^f Propofol plus, Zoetis UK Ltd, United Kingdom.

^g Isocare, Animalcare Ltd, United Kingdom.

^h Vivid E9, General Electric Medical Systems, Waukesha, Wisconsin.

ⁱ 4V-D Active Matrix 4D Volume Phased Array Transducer 1.5–4.0 MHz.

^j M5S-D Active Matrix single-crystal Phased Array Transducer 1.5–4.6 MHz.

^k EchoPAC PC versions 113, GE Healthcare, Horten, Norway.

^l Somatom Sensation 64, Siemens Medical Solutions, Erlangen, Germany.

^a Cardell Model 9402, CAS Medical Systems, Branford, Connecticut.

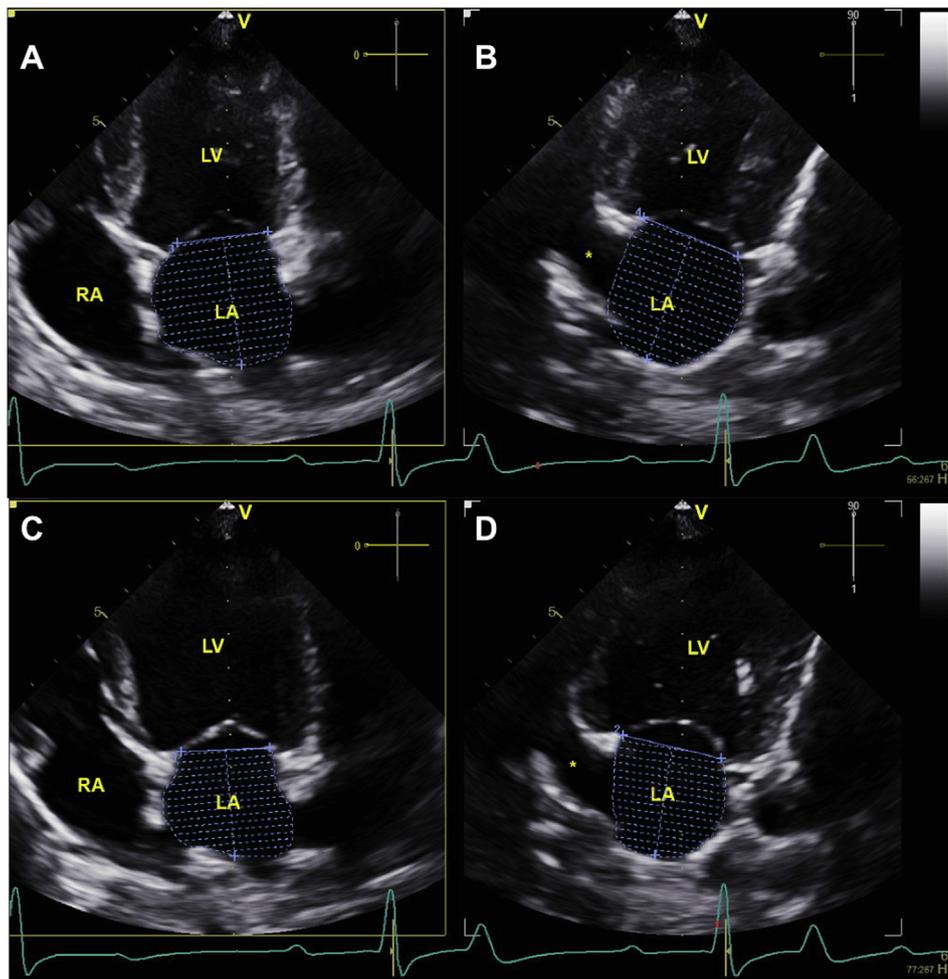


Figure 1 Representative real-time biplane echocardiography images of the left atrium just before mitral valve opening corresponding to maximum left atrial volume (A and B) and left atrium just after mitral valve closure corresponding to minimum left atrial volume (C and D) were obtained. The endocardial borders were traced manually while excluding the left auricular appendage (*) and the ostia of pulmonary veins, if visible. The mitral annulus was considered as the left atrioventricular border. The cut plane was adjusted from the left parasternal four-chamber view (A and C) in order to obtain a non-foreshortened two-chamber view (B and D). (A) Left parasternal four-chamber view (0°) when the left atrium is maximum. (B) Left parasternal two-chamber view (90°) when the left atrium is maximum. (C) Left parasternal four-chamber view (0°) when the left atrium is minimum. (D) Left parasternal two-chamber view (90°) when the left atrium is minimum. LA, left atrium; LV, left ventricle; RA, right atrium.

reconstruction interval, medium frequency reconstruction kernel, 80 kVp, 200 mA, 0.35 s tube rotation time and a collimator pitch of 0.51. Scan tube current was modulated by an automatic exposure control system^m. A premonitoring transverse scan was set at the level of the aortic arch, and the automated bolus tracking was set at 100 Hounsfield units with a cycle time of 3 s. A retrospectively ECG-gated cardiac MDCTA was performed using 700 mg I/kg of iodinated contrast

mediumⁿ followed by saline flush administered from a dual barrel injector^o at 5 mL/s and 325 psi. Scan parameters used for the retrospectively gated scan were set to 1.25-mm slice thickness, 0.625-mm spacing between slices, medium frequency reconstruction algorithm, field of view of 12 cm centred over the heart, 80 kVp, 400 mA, 0.35-s tube rotation time and collimator pitch of 0.24.

^m Care Dose 4D[®], Siemens Healthcare, Forchheim, Germany.

ⁿ Niopam 350[®], Bracco UK Ltd, United Kingdom.

^o Empower CTA^{®+}, Bracco[®] injeneering S.A., Milan, Italy.

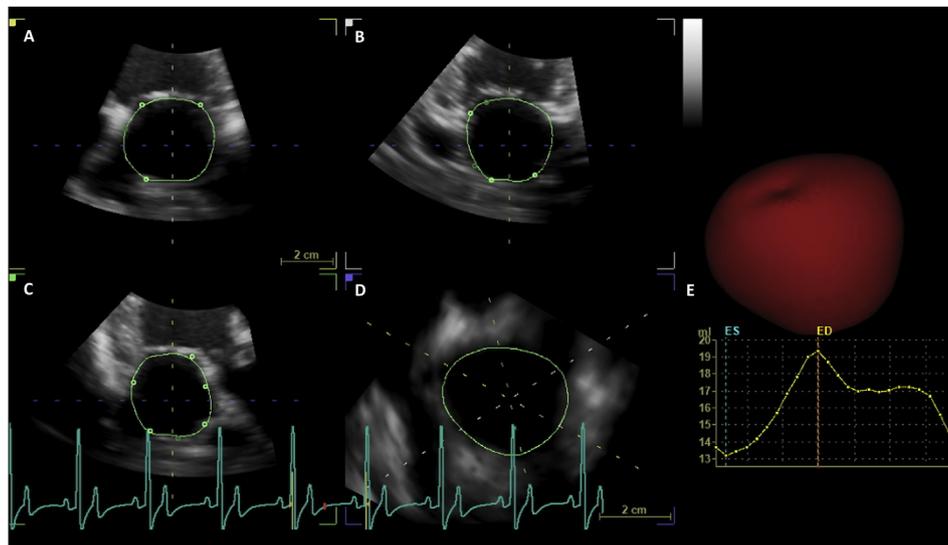


Figure 2 Representative real-time three-dimensional echocardiography images of the left atrium in a dog. After automatic slicing of real-time three-dimensional echocardiography data set and manual alignment, manual input for placing reference points was carried out (one point at the dorsal border of the left atrium, one point at the hinge-point of the septal leaflet and one point at the hinge-point of the lateral leaflet). Following this step, automatic detection of endocardial surface in three dimensions was generated. In this example, manual adjustment by adding a total of 3 points in left apical four-chamber view (A), 3 points in left apical two-chamber view (B) and 5 points in left apical five-chamber view (C) was performed. These manual adjustments permitted accurate delineation of the left atrium cavity prior volume measurement by the software. Left atrial cast associated to the time–volume curve (E) was obtained. Note that the electrocardiographic tracing at the lower edge of the image corresponds to the image just before mitral valve opening corresponding therefore to maximum left atrial volume. (A) Left apical four-chamber view. (B) Left apical two-chamber view. (C) Left apical five-chamber view. (D) Short-axis view of the left atrium. Note that the plane can be adjusted through a perpendicular axis from the roof of left atrium to the mitral valve annulus. (E) Automatically reconstructed three-dimensional left atrial cavity cast and its corresponding typical time–volume curve (y axis indicates left atrial volume [mL]; x-axis indicates time [s]). ED, end atrial diastole corresponding to maximum left atrial volume; ES, end atrial systole corresponding to minimum left atrial volume.

Measurement of LA size

Two-dimensional echocardiography

Angles of simultaneous multiplane 2D were adjusted to obtain left apical four- and two-chamber views that maximized LA size to avoid foreshortening. Images were optimized for endocardial visualization and temporal and spatial resolution using the focus, depth, sector size, frame rate, gain, compression, and time gain compensation controls. All measurements were performed at end-diastole (the frame just after mitral valve closure) and end-systole (just before mitral valve opening) to obtain LA_{min} and LA_{max} , respectively, according to the American Society of Echocardiography guidelines [10]. Care was taken to encompass the entire LA cavity in the data sets. The endocardial borders were traced manually

while excluding the left auricular appendage and the ostia of pulmonary veins, if visible (Fig. 1). The mitral annulus was considered as the left atrio-ventricular border. Three measurements were obtained and averaged for every dog.

Left atrial volume was calculated with the following formulae:

1) Area-length method calculation:

$$LAV = \frac{8}{3} \pi \frac{(A_{4c} \times A_{2c})}{L_{min}}$$

where A_{4c} is the area in the apical four-chamber view, A_{2c} is the area in the apical two-chamber view and L_{min} is the shorter length of the LA measured from the centre of the mitral annular plane to the superior border of the chamber.

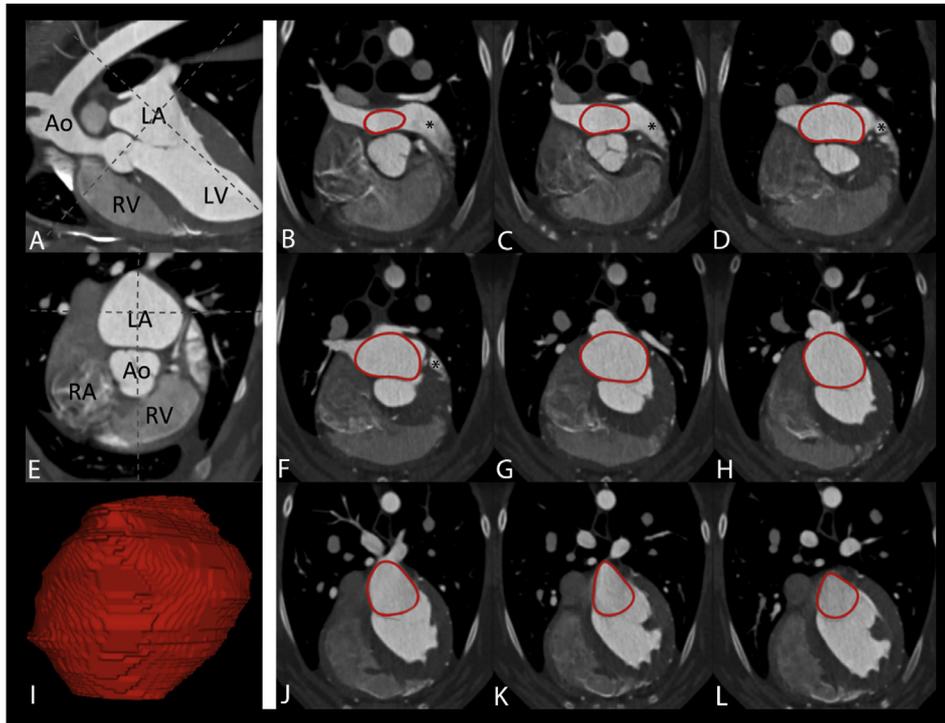


Figure 3 Cardiac electrocardiographic-gated multidetector computed tomography angiography in sagittal (A) and axial (E) planes. Regions of interest delineate the left atrium and extend from the dorsal border of the left atrium to the mitral valve annulus (B, C, D, F, G, H, J, K and L). Image I represents the computed three-dimensional volume. Ao, aorta; LA, left atrium; LV, left ventricle; RV, right ventricle. *Left auricle.

2) Method of disk calculation:

$$LAV = \frac{\pi}{4} \sum_{i=1}^n (Di4c)(Di2c) \frac{L}{n} hi$$

where h_i is the height of the stacked discs i and $Di4c$ and $Di2c$ are the two orthogonal minor and major axes derived from four- and two-chamber views, respectively.

Real-time three-dimensional echocardiography

Three-dimensional cine loops were acquired over eight consecutive cardiac cycles from the left parasternal view to obtain a single-beat full-volume data set with an average frame rate of 36.6 ± 10.3 frames per second (range 22.4–63 frames per second). Loops were digitally stored and analyzed offline with commercially available software^{k,p}. An effort was made to optimize image

quality, increasing the frame rate by narrowing the sector width and decreasing the depth. Maximum left atrial volume and LAV_{\min} were derived from semiautomated tracing of the LA endocardium at end ventricular systole and diastole, respectively. The software^{k,p} created an endocardial cast of the LA, according to reference points on the hinge-point of the septal leaflet, the hinge-points of the lateral leaflet and the dorsal border of the LA (Fig. 2, Supplemental video I, video available in Supplemental Material online). In all cases, the cast was manually adjusted so that the plane of the mitral valve defined one border, and the visual defect at the entry of the pulmonary veins was bridged. Care was taken to approximate the entire LA endocardial border frame by frame through the cardiac cycle. The pulmonary veins and left auricular appendage were not included. Three measurements were obtained and averaged for each dog from three representative cardiac cycles.

Electrocardiographic-gated MDCTA

All assessments and measurements were performed by a diagnostic imaging resident (F.T.) under board-certified veterinary radiologist (T.S.)

^p 4D-AutoLVQ, GE Healthcare, Horten, Norway.

Table 1 Descriptive statistics of left atrial volume during maximum and minimum left atrial size.

Variable	Mean	Standard deviation	Minimum	Maximum
LAV_{max} (mL)				
Biplane ALM	20.1	8.19	8.8	38.8
Biplane MOD	19.2	7.6	8.2	37.1
RT-3DE	15.1	6.2	7.1	29.4
MDCTA	16.0	6.7	7.2	31.5
LAV_{min} (mL)				
Biplane ALM	12.9	4.8	5.0	22.1
Biplane MOD	12.0	4.4	4.5	21.0
RT-3DE	9.4	3.8	3.3	15.9
MDCTA	10.1	4.21	3.3	17.6
LAV_{max} (mL/kg)				
Biplane ALM	0.63	0.31	0.29	1.43
Biplane MOD	0.68	0.34	0.32	1.55
RT-3DE	0.63	0.17	0.38	0.89
MDCTA	0.39	0.20	0.18	0.90
LAV_{min} (mL/kg)				
Biplane ALM	0.35	0.18	0.17	0.81
Biplane MOD	0.40	0.20	0.19	0.91
RT-3DE	0.39	0.11	0.25	0.56
MDCTA	0.19	0.09	0.09	0.43

ALM, area-length method; LAV_{max}, maximal left atrial volume; LAV_{min}, minimal left atrial volume; MDCTA, multi-detector computed tomography angiography; MOD, method of disk; RT-3DE, real-time three-dimensional echocardiography.

supervision, using dedicated DICOM viewer software^q. A window width of 1700 Hounsfield units and a window level of 200 Hounsfield units were used. The frames which depicted the LAV_{min} (just after mitral valve closure) and LAV_{max} (just before mitral valve opening) were subjectively determined on dynamic series using a 4D CINE mode review^q. This mode allows dynamic evaluation of a 3D image over time. Atrial volume analysis was performed by drawing regions of interest, delineating the LA border. Initially, two slices were drawn manually at each extremity of the LA, and the operator then drew slices between them at random locations. Subsequently, the software generated several interconnecting regions of interest (semiautomatic segmentation) that were adjusted manually to ensure accuracy. Finally, the software calculated LAV by summing the volumes of all the selected regions. The pulmonary veins

and left auricular appendage were not included. The anatomical limits of these structures were subjectively chosen by the operator based on the contour of the LA as part of the semiautomatic segmentation method (Fig. 3).

Variability analysis

To calculate intraobserver within-day and between-day variabilities, six echocardiograms and six MDCTA studies were randomly selected. Maximum left atrial volume and LAV_{min} were measured by every method (ALM, MOD, 3D volume derived from RT-3DE and ECG-gated MDCTA). The same cardiac cycle from the same cine loops of every echocardiogram and every ECG-gated MDCTA were subjected to repeated analyses by the same investigator (J.B. and F.T., respectively) at two different time points on a given day (morning and afternoon) and on two different days.

The same images were used to evaluate inter-observer variability. Two independent observers (Y.M.P. for echocardiography and J.B. for MDCTA) performed independent, blinded and repeated analyses.

Statistical analysis

A sample size of 20 observations per group was estimated to give >80% power to detect a correlation of at least 0.60 (with a critical p-value of 0.05) [33].

Statistical analyses were performed using commercially available software^{r,s,t}. Data were assessed for normality graphically and by use of the Shapiro–Wilk normality test. Continuous variables were reported as mean \pm standard deviation. Correlations (*r*) between echocardiographic techniques and MDCTA were determined by Pearson's correlation test and defined as excellent ($r \geq 0.90$), very good ($0.90 > r \geq 0.70$), good ($0.70 > r \geq 0.50$) or poor ($r < 0.50$) [34]. For sets of pairs of values, limits of agreement (LoA) and bias were assessed by Bland–Altman plots^r, to visualize the comparisons graphically. Analysis of agreement was performed using intraclass correlation coefficient (ICC), assessing consistency of single measurement with a two-way model (as all

^q OsiriX v5.8.5 64-bit, Geneva, Switzerland.

^r GraphPad Prism version 7.00 for Windows, GraphPad Software, La Jolla, California, USA.

^s Minitab 17, Pennsylvania, USA.

^t MedCalc Statistical Software, version 18.5, MedCalc Software bvba, Ostend, Belgium.

Table 2 Coefficient of variation for measurement of minimum left atrial volume and maximum left atrial volume according to different methods.

	LAV _{min} RT-3DE	LAV _{max} RT-3DE	LAV _{min} MOD	LAV _{max} MOD	LAV _{min} ALM	LAV _{max} ALM	LAV _{min} MDCTA	LAV _{max} MDCTA
CV interobserver (%)	6.45	4.82	14.8	5.73	13.87	7.67	4.86	7.27
CV within day (%)	1.48	1.67	3.41	3.99	3.59	4.43	2.97	3.51
CV between day (%)	2.31	1.69	4.10	3.85	3.99	4.19	5.70	2.74

ALM, area-length method; CV, coefficient of variation; LAV_{max}, maximal left atrial volume; LAV_{min}, minimal left atrial volume; MDCTA, multidetector computed tomography angiography; MOD, method of disk; RT-3DE, real-time three-dimensional echocardiography.

methods were used on all cases) and corresponding 95% confidence intervals (CIs), where 0–0.20 indicates poor agreement, 0.21–0.40 indicates fair agreement, 0.41–0.60 indicates moderate agreement, 0.61–0.80 indicates substantial agreement and >0.80 indicates almost perfect agreement.

These arbitrary cut-offs were similar to those used by Landis and Koch [35]. A p-value of less than 0.05 was considered to be statistically significant. Coefficients of variation were defined as the standard deviation of the differences divided by the mean of the variable under consideration and

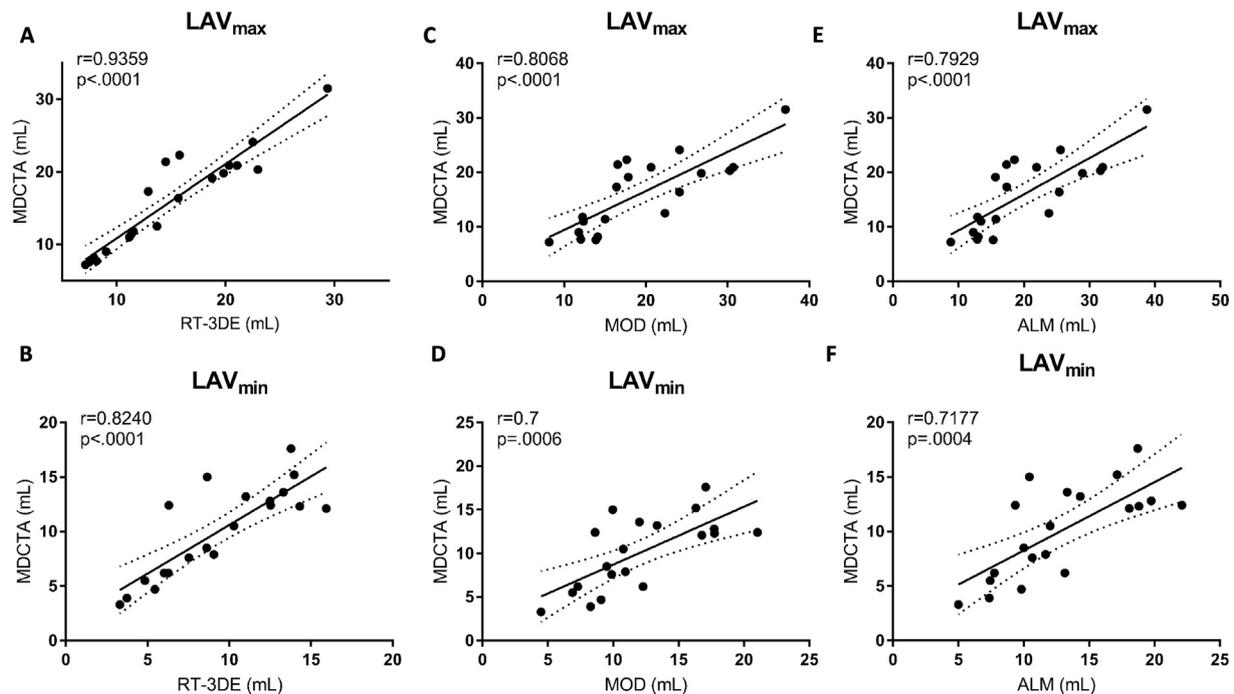


Figure 4 Correlations between RT-3DE, biplane MOD and biplane ALM with the reference method multidetector computed tomography angiography (MDCTA) for maximum left atrial volume (top) and minimum left atrial volume (bottom) of 20 anaesthetized dogs. When left atrial volume is maximal, there were positive correlations between MDCTA and RT-3DE ($r = 0.93$; $p < 0.0001$) (A), MDCTA and biplane MOD ($r = 0.81$; $p < 0.0001$) (C) and MDCTA and biplane ALM ($r = 0.79$; $p < 0.0001$) (E). Similarly, when left atrial volume is minimal, positive correlations were detected when comparing MDCTA and RT-3DE ($r = 0.82$; $p < 0.0001$) (B), MDCTA and biplane MOD ($r = 0.7$; $p = 0.0006$) (D) and MDCTA and biplane ALM ($r = 0.72$; $p = 0.0004$) (F). Solid lines represent the coefficient of correlation; dashed lines represent the 95% confidence intervals. Note that all methods correlate better for maximum left atrial volume. ALM, area-length method; LAV_{max}, maximal left atrial volume; LAV_{min}, minimal left atrial volume; MDCTA, multidetector computed tomography angiography; MOD, method of disk; RT-3DE, real-time three-dimensional echocardiography.

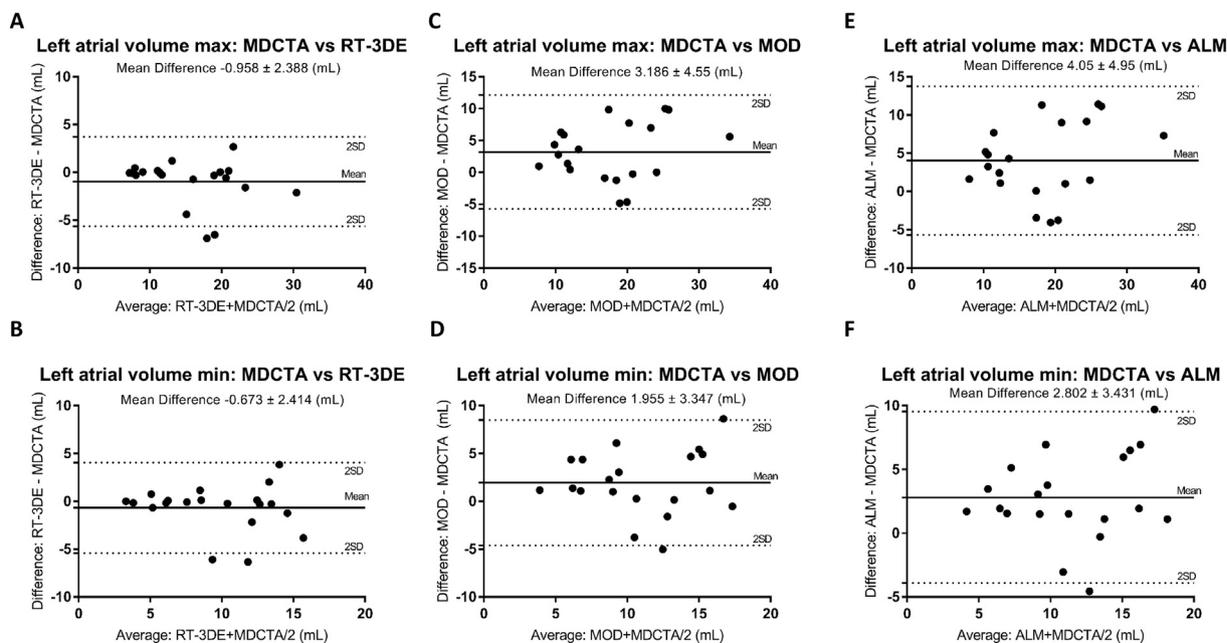


Figure 5 Bland–Altman analysis showing the agreement between maximal (top) and minimal (bottom) left atrial volumes measured by the reference method, multidetector computed tomography angiography, and those measured by RT-3DE (A and B), biplane MOD (C and D) or biplane ALM (E and F). Solid lines represent the mean difference (bias) and dashed lines represent the 95% limits of agreement (± 2 SD from the mean between the two techniques used). Note that MOD and ALM consistently overestimated left atrial volume, particularly at larger volume. By contrast, RT-3DE underestimated slightly left atrial volumes. ALM, area-length method; MDCTA, multidetector computed tomography angiography; MOD, method of disk; RT-3DE, real-time three-dimensional echocardiography; SD, standard deviation.

Table 3 Intraclass correlation coefficients and 95% CI reported for each part of measurements and for each parameter measured.

	LAV _{max} MDCTA	
	ICC	95% CI
LAV _{max} RT-3DE	0.9322	0.8371 to 0.9726
LAV _{max} ALM	0.7801	0.5244 to 0.9068
LAV _{max} MOD	0.8010	0.5635 to 0.9162
	LAV _{min} MDCTA	
	ICC	95% CI
LAV _{min} RT-3DE	0.8215	0.6032 to 0.9253
LAV _{min} ALM	0.7109	0.4017 to 0.8746
LAV _{min} MOD	0.6989	0.3815 to 0.8689

ALM, area-length method; CI, confidence interval; ICC, intraclass correlation; LAV_{max}, maximal left atrial volume; LAV_{min}, minimal left atrial volume; MDCTA, multidetector computed tomography angiography; MOD, method of disk; RT-3DE, real-time three-dimensional echocardiography. Coefficient interpretation: 0–0.2 indicates poor agreement; 0.3–0.4 indicates fair agreement; 0.5–0.7 indicates moderate agreement; 0.7–0.8 indicates strong agreement and >0.8 indicates almost perfect agreement.

were expressed as a percentage. Values < 15% were considered adequate for clinical use [36].

Results

The study population consisted of 20 dogs of various breeds including cross-breed (n = 4), Labrador retriever (n = 3), Golden retriever (n = 3), Cocker spaniel (n = 2) and one of each of the following breeds: Flat-coated retriever, schnauzer, Rough collie, samoyed, Northern inuit, English springer spaniel, boxer and a Border collie. There were four intact females, six neutered females, six neutered males and four intact males. The average age was 7.45 ± 4.14 years (range 0.6–14.3 years). The average weight was 26.3 ± 9.3 kg (range 9.1–44.5 kg) (supplemental Table A, data available in Supplemental Material online). Table 1 displays selected descriptive statistics for LAV_{max} and LAV_{min} according to the method used to calculate LAV. Coefficients of variation for within-day, between-day and interobserver variability of the four methods are listed in Table 2.

Real-time three-dimensional echocardiography and ECG-gated MDCTA

Left atrial volume by RT-3DE was highly correlated with MDCTA for LAV_{\max} ($r = 0.94$, $p < 0.0001$) and LAV_{\min} ($r = 0.82$, $p < 0.0001$) (Fig. 4A and B, respectively). However, on Bland–Altman analysis, RT-3DE slightly underestimated LAV_{\max} by 6% compared to MDCTA (bias = -0.96 mL, 95% LoA: $-5.6 - 3.7$; Fig. 5A). Similarly, RT-3DE underestimated LAV_{\min} by 6.7% (bias = -0.67 mL, 95% LoA: $-5.40 - 4.06$; Fig. 5B). Intraclass correlation (Table 3) confirmed these findings. There was almost perfect agreement between ECG-gated MDCTA and RT-3DE for LAV_{\max} (ICC = 0.93, CI: 0.83–0.97) and LAV_{\min} (ICC = 0.82, CI: 0.60–0.93).

Two-dimensional echocardiography and ECG-gated MDCTA

Two-dimensional echocardiographic assessment of LAV also correlated well with MDCTA but not as highly as RT-3DE (LAV_{\max} $r = 0.81$ [MOD] and 0.79 [ALM], both $p < 0.0001$, Fig. 4C and E and LAV_{\min} $r = 0.70$ [MOD] and 0.72 [ALM], $p < 0.0006$ and $p < 0.0004$ respectively, Fig. 4D and F). However, Bland–Altman analysis showed that MOD and ALM overestimated LAV_{\max} by 19.9% (bias = 3.18 mL, 95% LoA: $-5.7 - 12.1$) and 25.3% (bias = 4.05 mL, 95% LoA: $-5.6 - 13.7$), respectively (Fig. 5C and E). Minimum left atrial volume was also overestimated by 19.4% for MOD (bias = 1.96 mL, 95% LoA: $-4.6 - 8.5$) and 27.7% for ALM (bias = 2.80 mL, 95% LoA: $-3.9 - 9.5$) compared with MDCTA (Fig. 5D and F). The levels of agreement were less than those obtained by 3D imaging. Values obtained by 2D echocardiography also demonstrated substantial agreement with ECG-gated MDCTA for both LAV_{\max} (ALM; ICC = 0.78, CI: 0.52–0.91; MOD; ICC = 0.71, CI: 0.40–0.87) and LAV_{\min} (ALM; ICC = 0.80, CI: 0.56–0.92; MOD; ICC = 0.70, CI: 0.38–0.87).

Discussion

Real-time three-dimensional echocardiography is a new technique whose innovative use in people to quantify LAV has greatly expanded over the last decade. Multiple human studies have consistently shown that RT-3DE is a useful diagnostic tool that tends to underestimate LAV to a lesser extent than biplane ALM or MOD [12,13,24,27]. This is the first veterinary study to measure the degrees of accuracy and bias of a commercially available 3D

echocardiography system, using semiautomated border detection to measure LAV in a population of canine patients.

We have demonstrated that RT-3DE in dogs is more accurate at measuring LAV than 2D echocardiography when compared with the gold standard of 64-slice ECG-gated MDCTA. Real-time three-dimensional echocardiography-derived values were in almost perfect agreement with those obtained by MDCTA, whereas 2D methods overestimated LAV with wider LoA. In agreement with the recent work of Tidholm et al. [37], we conclude that 2D volume-based methods and RT-3DE cannot be used interchangeably to quantify LAV in dogs. Although 2D measurements remain easier and quicker to perform, RT-3DE is feasible, more accurate and highly reproducible, so that establishing canine reference ranges is a realistic goal.

We used an ECG-gated MDCTA volumetric gold standard because it is used to measure LAV in people with a high degree of accuracy, even when they have atrial fibrillation [24,25,38,39]. Furthermore, in dogs, ECG-gated MDCTA is already recognized as a volumetric gold standard for assessment of left and right ventricular volumes [40,41].

Accuracy of echocardiographic methods was determined in two stages. First, both RT-3DE and 2D echocardiography were shown to correlate highly with the volumetric gold standard. Second, Bland–Altman plots confirmed that RT-3DE outperformed 2DE with a minimal bias and the narrowest 95% LoA obtained for both LAV_{\max} and LAV_{\min} . The slight underestimation of RT-3DE that we recorded is consistent with reported biases in human medicine ranging from 0 to -2.5 mL [12,24].

Studies in people have consistently shown that 2D echocardiography, as well as RT-3DE, underestimates LAV compared to gold standard methods [12,13,15,20,24–27]. Surprisingly, in our study, we found that 2D planimetric methods overestimated LAV. The reason for this is unclear. It could be that differences in thoracic conformation and anatomical cardiac chamber anatomy mean that geometric assumptions that are valid in people do not apply to the canine LA [42]. Importantly, this discrepancy illustrates the pitfalls of extrapolating data across species when applying novel imaging modalities to veterinary medicine.

Two previous veterinary studies broadly agree with our data. They also demonstrated overestimation of LAV by both 2D planimetric methods, compared to RT-3DE [18] or cardiac magnetic resonance imaging [30], although cardiac magnetic resonance imaging does not appear to correlate

with monoplane MOD, RT-3DE or even MDCTA. Furthermore, and similar to people [22,43,44], our MOD-derived values were closer to MDCTA values than ALM-derived ones because biplane MOD makes fewer geometric assumptions than ALM [10]. This would suggest that in healthy dogs, although inferior to RT-3DE, biplane MOD remains the 2D planimetric method of choice for measuring LAV [10,37,43]. By contrast, in a recent Swedish study that included a large population of dogs with myxomatous mitral valve disease, biplane MOD underestimated LAV compared to RT-3DE [37]. Our data suggest that 2D geometric assumptions might be less accurate in dogs with bigger atria because there was a trend towards an increase in the scatter of the difference between MDCTA and planimetric measurements of LAV as atrial size increased.

Reduced accuracy at bigger LAV may relate to the views from which images were derived. Both RT-3DE and 2D images were obtained from left apical views. Apical imaging places LA in a far field of the ultrasound beam, leading to loss of lateral resolution, poor visualization and inaccurate tracing of the LA endocardial border [22,45]. Despite significant effort by the sonographer to obtain good quality non-foreshortened four- and two-chamber views by optimizing the width and the depth, manual tracing errors may have contributed to LAV overestimation by including some of the LAA or pulmonary veins [46]. Indeed, unlike in people, canine pulmonary veins anastomose into a cone-shaped trunk prior to entering the LA. This leads to an imprecise delineation between LA tissue and the beginning of pulmonary veins [42]. By contrast, in RT-3DE, we used semiautomated software package designed to provide an ellipsoidal 3D cast of the left ventricle after placing three reference points on the endocardial border. Although this required manual adjustment, the degree of manual involvement was significantly less than that with 2D techniques. It is possible that the software package is superior to manual selection of border delineation, resulting in greater inaccuracy where there is greater manual input, i.e. 2D methods. Indeed, manual tracing of the endocardium is operator dependant and tends to be associated with higher interobserver variability than RT-3DE [20]. Despite the reproducibility among the echocardiographic methods in our study being <15%, and hence clinically acceptable compared to previously reported human [12,20,24] and veterinary [18,43,47] studies, the effect size would be greater with bigger LA, which have longer perimeters. We conclude that despite the advantages of RT-3DE over 2D

imaging, RT-3DE requires separate validation for measuring LAV in disease states, using a large population of dogs.

These findings are clinically significant because thoracic conformation can vary greatly in dogs of different morphotypes potentially leading to anatomical variation, including LAV [48,49]. Indeed, Hollmer et al. [47] have documented significant breed-related differences in LAV using the biplane ALM in dogs with normal cardiovascular status. By contrast, we demonstrated that RT-3DE maintained its bias over a range of LAV within brachycephalic, dolichocephalic and mesaticephalic breeds with slight underestimation. We speculate that RT-3DE would also demonstrate the same bias and degree of accuracy within breeds over a range of pathological LA remodelling. Additional research validating the use of RT-3DE measurements in dogs with enlarged LA is warranted to confirm this hypothesis.

Our study has several noteworthy limitations that should be considered. It was not designed to correct for potential confounders such as heart rate, changes in LA loading conditions, sex, image quality and eventually variability throughout the breathing cycle, and no attempts were made to correlate these parameters with LAV. Sporadically, we found that sinus arrhythmia or heart rates greater than 80 beats per minute caused stair-step and motion artefacts on MDCTA. This was due to the limited temporal resolution of 64-slice ECG-gated MDCTA and the absence of breath-holding during data acquisition. The consequence was poorer definition of the LA endocardial border, although we believe that this was not sufficient to lead to erroneous measurements because each patient served as his own control with short time-frame between modalities and therefore data acquisitions.

The confounding effects on respirophasic changes are likely to have been similar between the different methods used to measure LAV [50]. Lung expansion during end-inspiration decreases LAV, and conversely, LAV increases during end-expiration [50,51]. In our study, anaesthetized dogs were assisted by mechanical ventilation during both MDCTA and echocardiography. Image acquisition was not synchronised with the breathing cycle, which could theoretically influence the loading condition of the LA. Synchronization with the breathing cycle would have implied using breath-holding, which was not undertaken not only for ethical reasons but also to mirror clinical situations. Besides, breath-holding could have influenced the loading of the LA by up to 20% compared to normal breathing [52].

Real-time three-dimensional echocardiography is also subject to limited temporal and spatial resolution during real-time acquisition. In previous veterinary studies, the optimal balance between spatial and temporal resolution was obtained by acquiring volume data sets with multibeat modalities involving acquisition of four to seven cardiac cycles [16–18,53]. However, to avoid stitching artefact, this mode requires a regular heart rate (ideally between 60 and 90 beats per minute based on the author experience), breath-holding and stable probe handling from the operator. This is not easily achieved in a clinical veterinary setting. Our aim was to demonstrate the clinical feasibility of RT-3DE, and because inhalation anaesthetics can increase the heart rate by decreasing cardiac vagal activity [54], single-beat acquisition was preferred at the expense of image quality. Overall image quality was deemed adequate for LAV estimation, and our conclusions should be equally applicable to emerging 3D technologies with improved image quality.

It is also worth emphasizing that frame selection varied due to image quality and frame rate. Consequently, measurements were not performed at exactly the same time point, potentially leading to underestimation of LA. However, we attempted to overcome this limitation by relying on the average of three different measurements for each variable for both MDCTA and RT-3DE.

The aim of this study was not to generate allometric relationships in order to establish reference values for RT-3DE and planimetric methods. Additional studies involving the use of RT-3DE in a larger population of dogs are required to establish reference values in healthy and conscious patients and to optimize the clinical utility of RT-3DE to estimate LAV.

Conclusions

This is the first prospective study in veterinary medicine to study the accuracy and the bias of RT-3DE with a volumetric gold standard to estimate LAV. Three-dimensionally derived LAV measurements were found to be feasible, reproducible and more accurate than 2D echocardiography-based volumetric methods. Our results might facilitate future clinical research in order to determine a general consensus for the best method to assess LAV. Although RT-3DE is not currently widely available in veterinary medicine, this modality remains appealing and holds promise for LAV assessment. It is anticipated that this imaging modality will emerge as a powerful diagnostic tool

and will be integrated into clinical guidelines and routine practice as the imaging modality of choice for LA assessment with dedicated software and adapted algorithms alongside the improvement of spatial and temporal resolution in the next generation of 3D probes.

Conflicts of interest statement

The authors do not have any conflicts of interest to disclose.

Supplementary data

Supplementary data to this article can be found online at <https://doi.org/10.1016/j.jvc.2019.06.004>.

References

- [1] Borgarelli M, Santilli RA, Chiavegato D, D'Agnolo G, Zanatta R, Mannelli A, Tarducci A. Prognostic indicators for dogs with dilated cardiomyopathy. *J Vet Intern Med* 2006; 20:104–10.
- [2] Borgarelli M, Savarino P, Crosara S, Santilli RA, Chiavegato D, Poggi M, Bellino C, La Rosa G, Zanatta R, Haggstrom J, Tarducci A. Survival characteristics and prognostic variables of dogs with mitral regurgitation attributable to myxomatous valve disease. *J Vet Intern Med* 2008;22:120–8.
- [3] Rossi A, Cicoira M, Zanolla L, Sandrini R, Golia G, Zardini P, Enriquez-Sarano M. Determinants and prognostic value of left atrial volume in patients with dilated cardiomyopathy. *J Am Coll Cardiol* 2002;40:1425–30.
- [4] Sargent J, Muzzi R, Mukherjee R, Somarathne S, Schranz K, Stephenson H, Connolly D, Brodbelt D, Luis Fuentes V. Echocardiographic predictors of survival in dogs with myxomatous mitral valve disease. *J Vet Cardiol* 2015;17:1–12.
- [5] Wu VC-C, Takeuchi M, Kuwaki H, Iwataki M, Nagata Y, Otani K, Haruki N, Yoshitani H, Tamura N, Abe H, Negishi K, Lin FC, Otsuji Y. Prognostic value of LA volumes assessed by transthoracic 3D echocardiography. *J Am Coll Cardiol Img* 2013;6:1025–35.
- [6] Rishniw M, Erb HN. Evaluation of four 2-dimensional echocardiographic methods of assessing left atrial size in dogs. *J Vet Intern Med* 2000;14:429–35.
- [7] Hansson K, Haggstrom J, Kwart C, Lord P. Left atrial to aortic root indices using two-dimensional and M-mode echocardiography in cavalier King Charles spaniels with and without left atrial enlargement. *Vet Radiol Ultrasound* 2002;43:568–75.
- [8] De Madron É. Normal echocardiographic values. In: De Madron É, Chetboul V, Bussadori C, editors. *Clinical Echocardiography of the Dog and Cat*. St. Louis: Elsevier; 2015. p. 21–37.
- [9] Wesselowski S, Borgarelli M, Bello NM, Abbott J. Discrepancies in identification of left atrial enlargement using left

- atrial volume versus left atrial-to-aortic root ratio in dogs. *J Vet Intern Med* 2014;28:1527–33.
- [10] Lang RM, Badano LP, Mor-Avi V, Afilalo J, Armstrong A, Ernande L, Flachskampf FA, Foster E, Goldstein SA, Kuznetsova T, Lancellotti P, Muraru D, Picard MH, Rietzschel ER, Rudski L, Spencer KT, Tsang W, Voigt J-U. Recommendations for cardiac chamber quantification by echocardiography in adults: an update from the American society of echocardiography and the European association of cardiovascular imaging. *Eur Hear J Cardiovasc Imaging* 2015;16:233–71.
 - [11] Vizzardi E, D'Aloia A, Rocco E, Lupi L, Rovetta R, Quinzani F, Bontempi L, Curnis A, Dei Cas L. How should we measure left atrium size and function? *J Clin Ultrasound* 2012;40:155–66.
 - [12] Mor-Avi V, Yodwut C, Jenkins C, Kühl H, Nesser H-J, Marwick TH, Franke A, Weinert L, Niel J, Steringer-Mascherbauer R, Free BH, Sugeng L, Lang R. Real-time 3D echocardiographic quantification of left atrial volume. *J Am Coll Cardiol Img* 2012;5:769–77.
 - [13] Koka AR, Gould SD, Owen AN, Halpern EJ. Left atrial volume: comparison of 2D and 3D transthoracic echocardiography with ECG-gated CT angiography. *Acad Radiol* 2012;19:62–8.
 - [14] Maddukuri PV, Vieira MLC, DeCastro S, Maron MS, Kuvin JT, Patel AR, Pandian NG. What is the best approach for the assessment of left atrial size? Comparison of various unidimensional and two-dimensional parameters with three-dimensional echocardiographically determined left atrial volume. *J Am Soc Echocardiogr* 2006;19:1026–32.
 - [15] Al-Mohaisen MA, Kazmi MH, Chan KL, Chow BJW. Validation of two-dimensional methods for left atrial volume measurement: a comparison of echocardiography with cardiac computed tomography. *Echocardiography* 2013;30:1135–42.
 - [16] Tidholm A, Bodegård-Westling A, Höglund K, Ljungvall I, Häggström J. Comparisons of 2- and 3-dimensional echocardiographic methods for estimation of left atrial size in dogs with and without myxomatous mitral valve disease. *J Vet Intern Med* 2011;25:1320–7.
 - [17] Tidholm A, Höglund K, Häggström J, Bodegård-Westling A, Ljungvall I. Left atrial ejection fraction assessed by real-time 3-dimensional echocardiography in normal dogs and dogs with myxomatous mitral valve disease. *J Vet Intern Med* 2013;27:884–9.
 - [18] LeBlanc N, Scollan K, Sisson D. Quantitative evaluation of left atrial volume and function by one-dimensional, two-dimensional, and three-dimensional echocardiography in a population of normal dogs. *J Vet Cardiol* 2016;18:336–49.
 - [19] Jenkins C, Bricknell K, Marwick TH. Use of Real-time Three-dimensional echocardiography to measure left atrial volume: comparison with other echocardiographic techniques. *J Am Soc Echocardiogr* 2005;18:991–7.
 - [20] Badano LP, Miglioranza MH, Mihăilă S, Peluso D, Xhaxho J, Marra MP, Cucchini U, Soriani N, Iliceto S, Muraru D. Left atrial volumes and function by three-dimensional echocardiography. *Circ Cardiovasc Imaging* 2016;9:e004229.
 - [21] Gweon HM, Kim SJ, Kim TH, Lee SM, Hong YJ, Rim S-J. Evaluation of left atrial volumes using multidetector computed tomography: comparison with echocardiography. *Korean J Radiol* 2010;11:286.
 - [22] Takagi Y, Ehara S, Okuyama T, Shirai N, Yamashita H, Sugioka K, Kitamura H, Ujino K, Hozumi T, Yoshiyama M. Comparison of determinations of left atrial volume by the biplane area-length and Simpson's methods using 64-slice computed tomography. *J Cardiol* 2009;53:257–64.
 - [23] Mahabadi AA, Samy B, Seneviratne SK, Toepker MH, Bamberg F, Hoffmann U, Truong QA. Quantitative assessment of left atrial volume by electrocardiographic-gated contrast-enhanced multidetector computed tomography. *J Cardiovasc Comput Tomogr* 2009;3:80–7.
 - [24] Miyasaka Y, Tsujimoto S, Maeba H, Yuasa F, Takehana K, Dote K, Iwasaka T. Left atrial volume by real-time three-dimensional echocardiography: validation by 64-slice multidetector computed tomography. *J Am Soc Echocardiogr* 2011;24:680–6.
 - [25] Kühl JT, Lønborg J, Fuchs A, Andersen MJ, Vejlsstrup N, Kelbæk H, Engstrøm T, Møller JE, Kofoed K. Assessment of left atrial volume and function: a comparative study between echocardiography, magnetic resonance imaging and multi slice computed tomography. *Int J Cardiovasc Imaging* 2012;28:1061–71.
 - [26] Rodevand O, Bjornerheim R, Ljosland M, Maehle J, Smith HJ, Ihlen H. Left atrial volumes assessed by three- and two-dimensional echocardiography compared to MRI estimates. *Int J Cardiovasc Imaging* 1999;15:397–410.
 - [27] Artang R, Migrino RQ, Harmann L, Bowers M, Woods TD. Left atrial volume measurement with automated border detection by 3-dimensional echocardiography: comparison with magnetic resonance imaging. *Cardiovasc Ultrasound* 2009;7:16.
 - [28] Chin RB, Tighe C, Beaver T, Welch T, Costa S. Advances in 3D echocardiography: automated software improves the learning curve and clinical implementation in a real world setting for quantitative assessment of left ventricular ejection. *J Am Coll Cardiol* 2017;69:1642.
 - [29] Tsang W, Salgo IS, Medvedofsky D, Takeuchi M, Prater D, Weinert L, Yamat M, Mor-Avi V, Patel A, Lang R. Transthoracic 3D echocardiographic left heart chamber quantification using an automated adaptive analytics algorithm. *J Am Coll Cardiol Img* 2016;9:769–82.
 - [30] Fries RC, Gordon SG, Saunders AB, Miller MW, Hariu CD, Schaeffer DJ. Quantitative assessment of two- and three-dimensional transthoracic and two-dimensional transesophageal echocardiography, computed tomography, and magnetic resonance imaging in normal canine hearts. *J Vet Cardiol* 2019;21:79–92.
 - [31] Thomas WP, Gaber CE, Jacobs GJ, Kaplan PM, Lombard CW, Moise NS, Moses BL. Recommendations for standards in transthoracic two-dimensional echocardiography in the dog and cat. Echocardiography committee of the specialty of cardiology, American College of veterinary internal medicine. *J Vet Intern Med* 1993;7:247–52.
 - [32] Quiñones MA, Otto CM, Stoddard M, Waggoner A, Zoghbi WA. Recommendations for quantification of Doppler echocardiography: a report from the Doppler quantification task force of the nomenclature and standards committee of the American Society of Echocardiography. *J Am Soc Echocardiogr* 2002;15:167–84.
 - [33] Browner WS, Newman TB, Hulley SB. Estimating sample size and power: applications and examples. In: Hulley SB, Cummings SR, Browner WS, Grady D, Newman TB, editors. *Designing Clinical Research: An Epidemiologic Approach*. 4th ed. Philadelphia: Lippincott Williams & Wilkins; 2013. p. 79. appendix 6C.
 - [34] Hinkle DE, Wiersma W, Jurs SG. Rule of thumb for interpreting the size of a correlation coefficient. In: Hinkle DE, Wiersma W, Jurs SG, editors. *Applied Statistics for the Behavioral Sciences*. 5th ed. Boston: Houghton Mifflin; 2003.
 - [35] Landis JR, Koch GG. The measurement of observer agreement for categorical data. *Biometrics* 1977;33:159–74.

- [36] Chetboul V. Intra- and interoperator variability. In: De Madron É, Chetboul V, Bussadori C, editors. *Clinical Echocardiography of the Dog and Cat*. St. Louis: Elsevier; 2015. p. 39–43.
- [37] Tidholm A, Bodegård-Westling A, Höglund K, Häggström J, Ljungvall I. Comparison between real-time 3-dimensional and 2-dimensional biplane echocardiographic assessment of left atrial volumes in dogs with myxomatous mitral valve disease. *J Vet Intern Med* 2019;33:455–61.
- [38] Agner BFR, Kühl JT, Linde JJ, Kofoed KF, Akesson P, Rasmussen BV, Jensen GB, Dixen U. Assessment of left atrial volume and function in patients with permanent atrial fibrillation: comparison of cardiac magnetic resonance imaging, 320-slice multi-detector computed tomography, and transthoracic echocardiography. *Eur Heart J Cardiovasc Imaging* 2014;15:532–40.
- [39] Rohner A, Brinkert M, Kawel N, Buechel RR, Leibundgut G, Grize L, Kühne M, Bremerich J, Kaufmann BA, Zellweger MJ, Buser P, Osswald S, Handke M. Functional assessment of the left atrium by real-time three-dimensional echocardiography using a novel dedicated analysis tool: initial validation studies in comparison with computed tomography. *Eur Heart J Cardiovasc Imaging* 2011;12:497–505.
- [40] Scollan KF, Stieger-Vanegas SM, Sisson DD. Assessment of left ventricular volume and function in healthy dogs by use of one-, two-, and three-dimensional echocardiography versus multidetector computed tomography. *Am J Vet Res* 2016;77:1211–9.
- [41] Sieslack AK, Dziallas P, Nolte I, Wefstaedt P, Hungerbühler SO. Quantification of right ventricular volume in dogs: a comparative study between three-dimensional echocardiography and computed tomography with the reference method magnetic resonance imaging. *BMC Vet Res* 2014;10:242.
- [42] Brewer FC, Moïse NS, Kornreich BG, Bezuidenhout AJ. Use of computed tomography and silicon endocasts to identify pulmonary veins with echocardiography. *J Vet Cardiol* 2012;14:293–300.
- [43] Höllmer M, Willesen JL, Tolver A, Koch J. Comparison of four echocardiographic methods to determine left atrial size in dogs. *J Vet Cardiol* 2016;18:137–45.
- [44] Jiamsripong P, Honda T, Reuss C, Hurst R, Chaliki H, Grill D, Schnek SL, Tyler R, Khandheria BK, Lester SJ. Three methods for evaluation of left atrial volume. *Eur J Echocardiogr* 2007;9:351–5.
- [45] Lester SJ, Ryan EW, Schiller NB, Foster E. Best method in clinical practice and in research studies to determine left atrial size. *Am J Cardiol* 1999;84:829–32.
- [46] Russo C, Hahn RT, Jin Z, Homma S, Sacco RL, Di Tullio MR. Comparison of echocardiographic single-plane versus biplane method in the assessment of left atrial volume and validation by real time three-dimensional echocardiography. *J Am Soc Echocardiogr* 2010;23:954–60.
- [47] Höllmer M, Willesen JL, Tolver A, Koch J. Left atrial volume and phasic function in clinically healthy dogs of 12 different breeds. *Vet J* 2013;197:639–45.
- [48] Evans EH, De Lahunta A. The skeleton. In: Evans EH, De Lahunta A, editors. *Miller's Anatomy of the Dog*. 4th ed. St. Louis, MO: Saunders; 2013. p. 86–7.
- [49] Schwarz T, Sullivan M, Hartung K. Radiographic anatomy of the cribiform plate (lamina cribrosa). *Vet Radiol Ultrasound* 2000;41:220–5.
- [50] Sørgaard M, Linde JJ, Ismail H, Risum N, Kofoed KF, Kühl JT, Tittle B, Nielsen WB, Hove JD. Respiratory influence on left atrial volume calculation with 3D-echocardiography. *Cardiovasc Ultrasound* 2016;14:11.
- [51] Riddervold F, Smiseth OA, Risoe C. The effect of positive end-expiratory pressure ventilation on atrial filling. *Acta Anaesthesiol Scand* 1991;35:448–52.
- [52] Poutanen T. Left atrial volume assessed by transthoracic three dimensional echocardiography and magnetic resonance imaging: dynamic changes during the heart cycle in children. *Heart* 2000;83:537–42.
- [53] Tidholm A, Bodegård-Westling A, Höglund K, Häggström J, Ljungvall I. Real-time 3-dimensional echocardiographic assessment of effective regurgitant orifice area in dogs with myxomatous mitral valve disease. *J Vet Intern Med* 2017;31:303–10.
- [54] Picker O, Scheeren TWL, Arndt JO. Inhalation anaesthetics increase heart rate by decreasing cardiac vagal activity in dogs. *Br J Anaesth* 2001;87:748–54.